



CAS

# Beam Diagnostics

## Lecture 1

Uli Raich  
CERN BE - BI  
(Beam Instrumentation)



# Overview






- First hour:
  - Introduction
  - Overview of measurement instruments
    - Faraday Cup
    - Beam Current Transformer
    - Beam Position Monitor
    - Profile Detectors
      - SEMGrids
      - Wire Scanners
    - Beam Loss Monitors
- Second hour
  - Some depicted examples of beam parameter measurements



# Introduction

# CAS

**An accelerator can never be better than the instruments measuring its performance!**

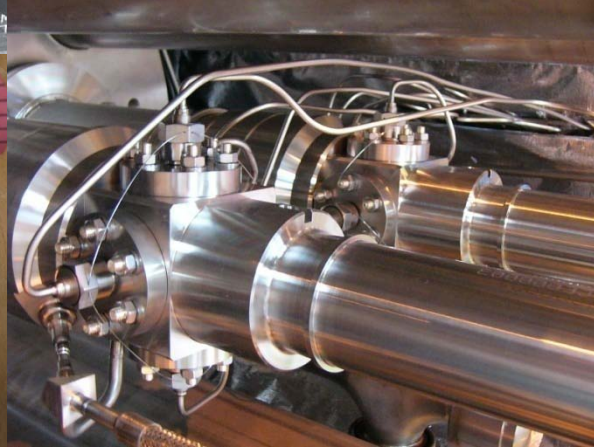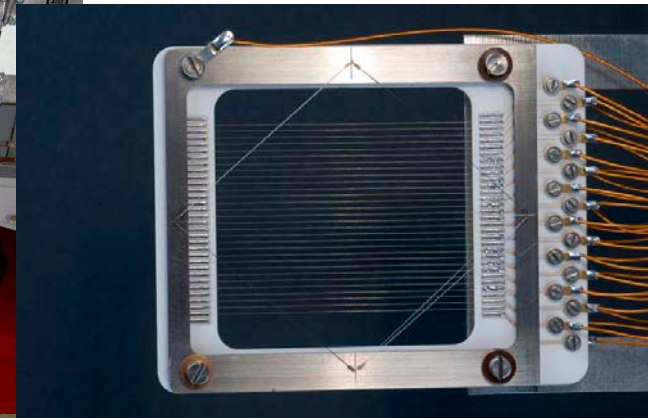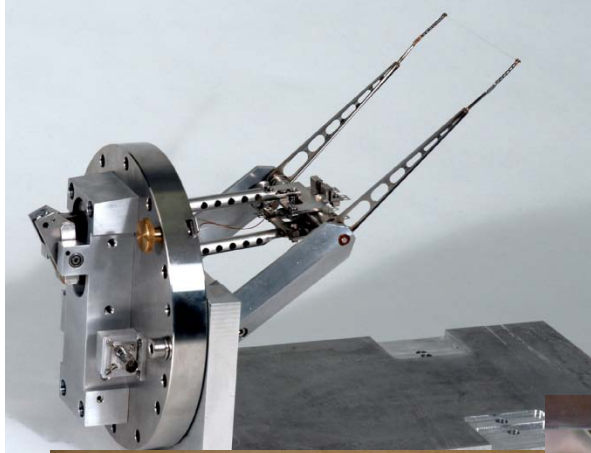



# Different uses of beam diagnostics



- **Regular crude checks of accelerator performance**
  - Beam Intensity
  - Radiation levels
- **Standard regular measurements**
  - Emittance measurement
  - Trajectories
  - Tune
- **Sophisticated measurements e.g. during machine development sessions**
  - May require offline evaluation
  - May be less *comfortable*





# Diagnostic devices and quantity measured





<b>Instrument</b>	<b>Physical Effect</b>	<b>Measured Quantity</b>	<b>Effect on beam</b>
<b>Faraday Cup</b>	<b>Charge collection</b>	<b>Intensity</b>	<b>Destructive</b>
<b>Current Transformer</b>	<b>Magnetic field</b>	<b>Intensity</b>	<b>Non destructive</b>
<b>Wall current monitor</b>	<b>Image Current</b>	<b>Intensity</b> <b>Longitudinal beam shape</b>	<b>Non destructive</b>
<b>Pick-up</b>	<b>Electric/magnetic field</b>	<b>Position</b>	<b>Non destructive</b>
<b>Secondary emission monitor</b>	<b>Secondary electron emission</b>	<b>Transverse size/shape, emittance</b>	<b>Disturbing, can be destructive at low energies</b>
<b>Wire Scanner</b>	<b>Secondary particle creation</b>	<b>Transverse size/shape</b>	<b>Slightly disturbing</b>
<b>Scintillator screen</b>	<b>Atomic excitation with light emission</b>	<b>Transverse size/shape (position)</b>	<b>Destructive</b>
<b>Residual Gas monitor</b>	<b>Ionization</b>	<b>Transverse size/shape</b>	<b>Non destructive</b>



# A beam parameter measurement

CAS

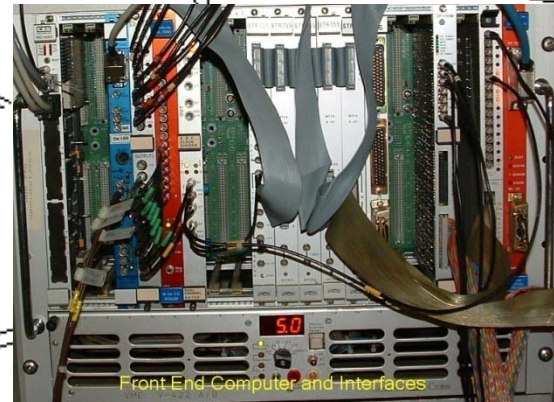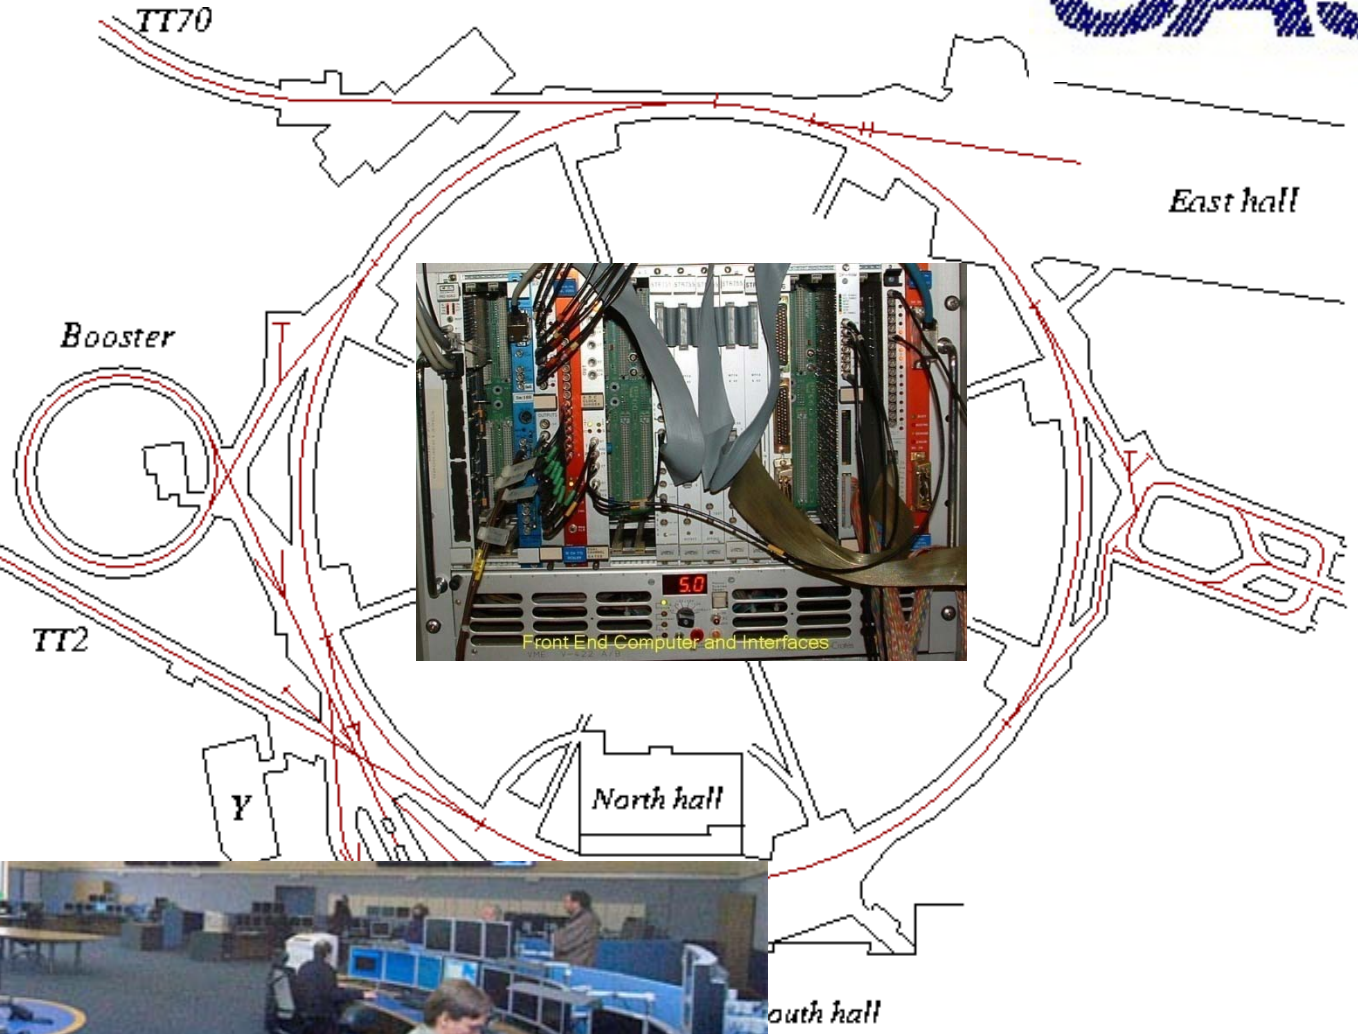



## Required Competence in a beam diagnostics group




- Some beam physics in order to understand the beam parameters to be measured and to distinguish beam effects from sensor effects
- Detector physics to understand the interaction of the beam with the sensor
- Mechanics
- Analogue signal treatment
  - Low noise amplifiers
  - High frequency analogue electronics
- Digital signal processing
- Digital electronics for data readout
- Front-end and Application Software



# Layout of a Faraday Cup

CAS



- Electrode: 1 mm stainless steel
- Only low energy particles can be measured
- Very low intensities (down to 1 pA) can be measured
- Creation of secondary electrons of low energy (below 20 eV)
- Repelling electrode with some 100 V polarisation voltage pushes secondary electrons back onto the electrode

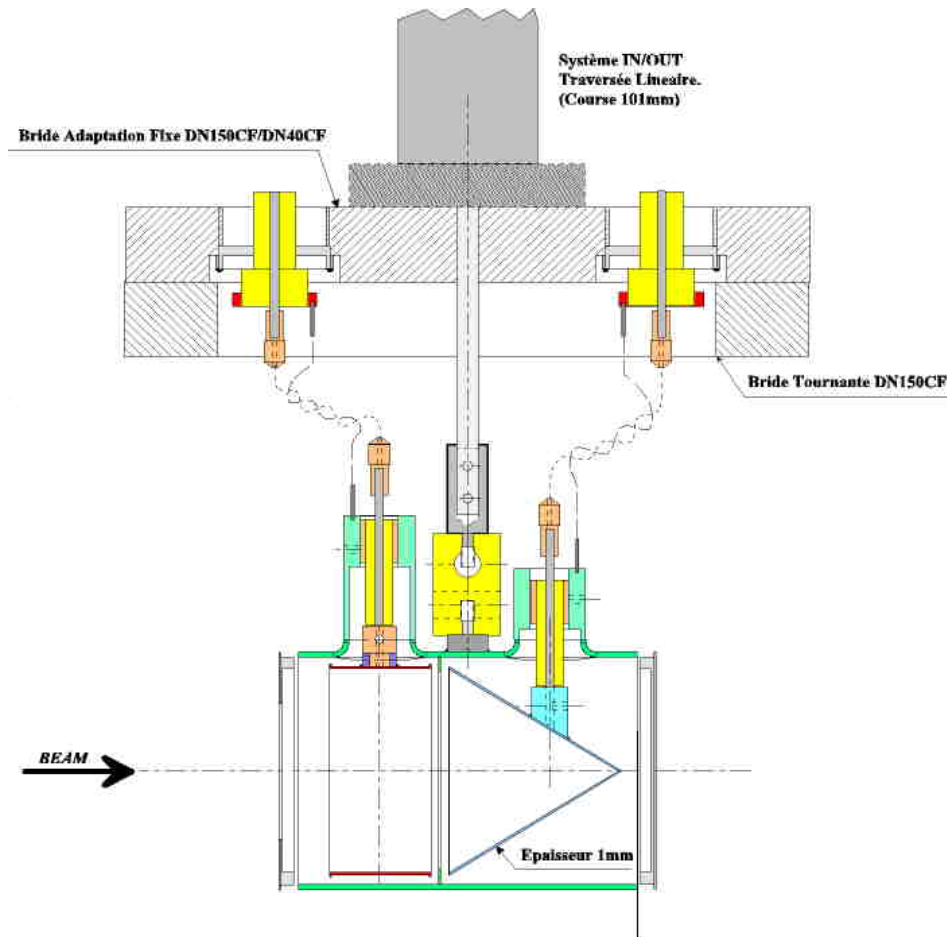



# Faraday Cup

CAS

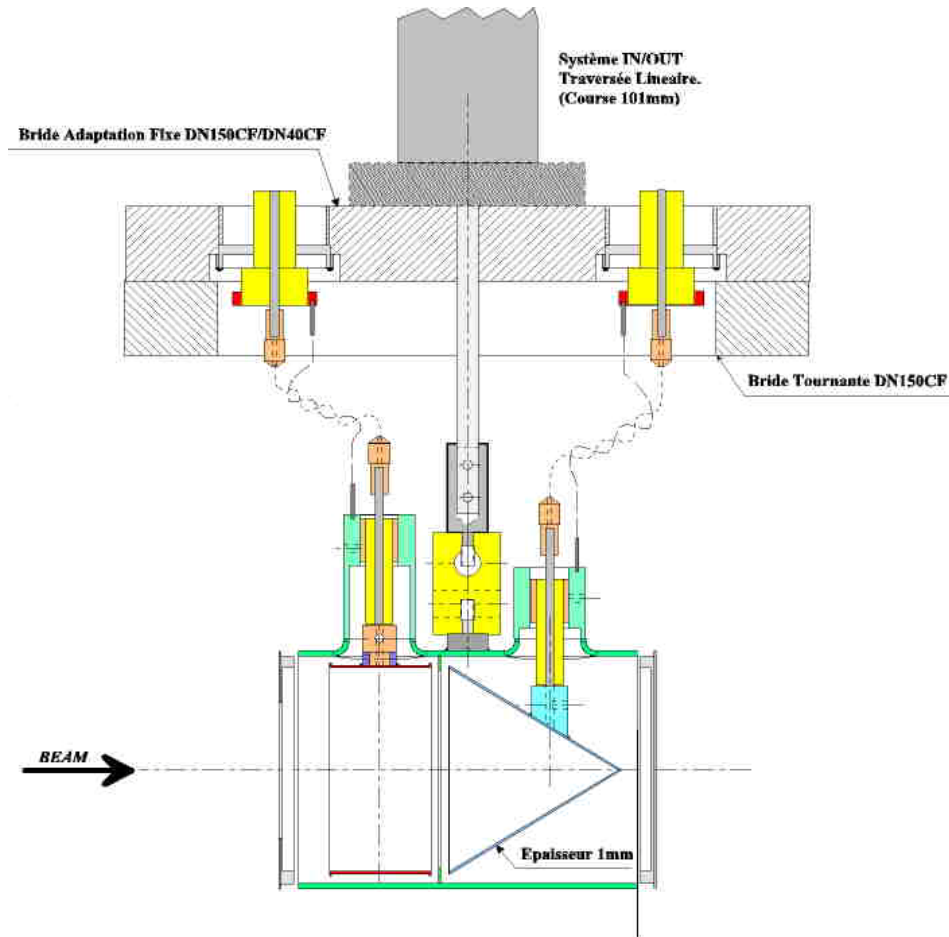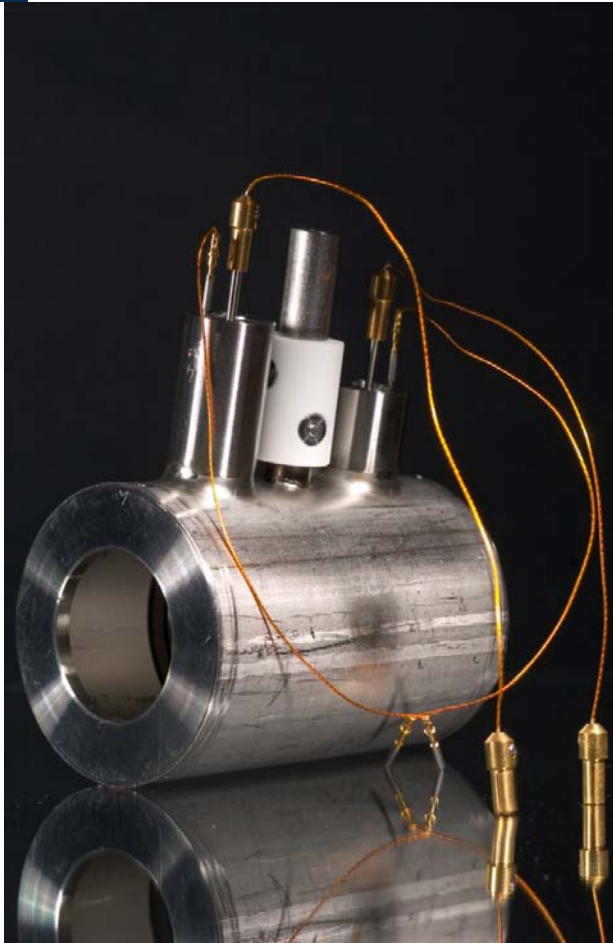






# Electro-static Field in Faraday Cup

CAS

In order to keep secondary electrons with the cup a repelling voltage is applied to the polarization electrode

Since the electrons have energies of less than 20 eV some 100V repelling voltage is sufficient

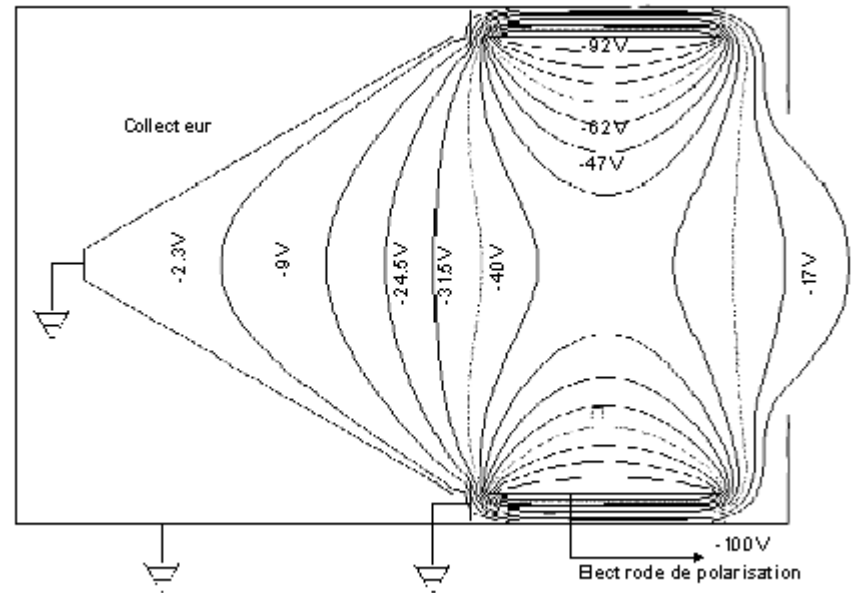




# Energy of secondary emission electrons


CAS

- With increasing repelling voltage the electrons do not escape the Faraday Cup any more and the current measured stays stable.
- At 40V and above no decrease in the Cup current is observed any more

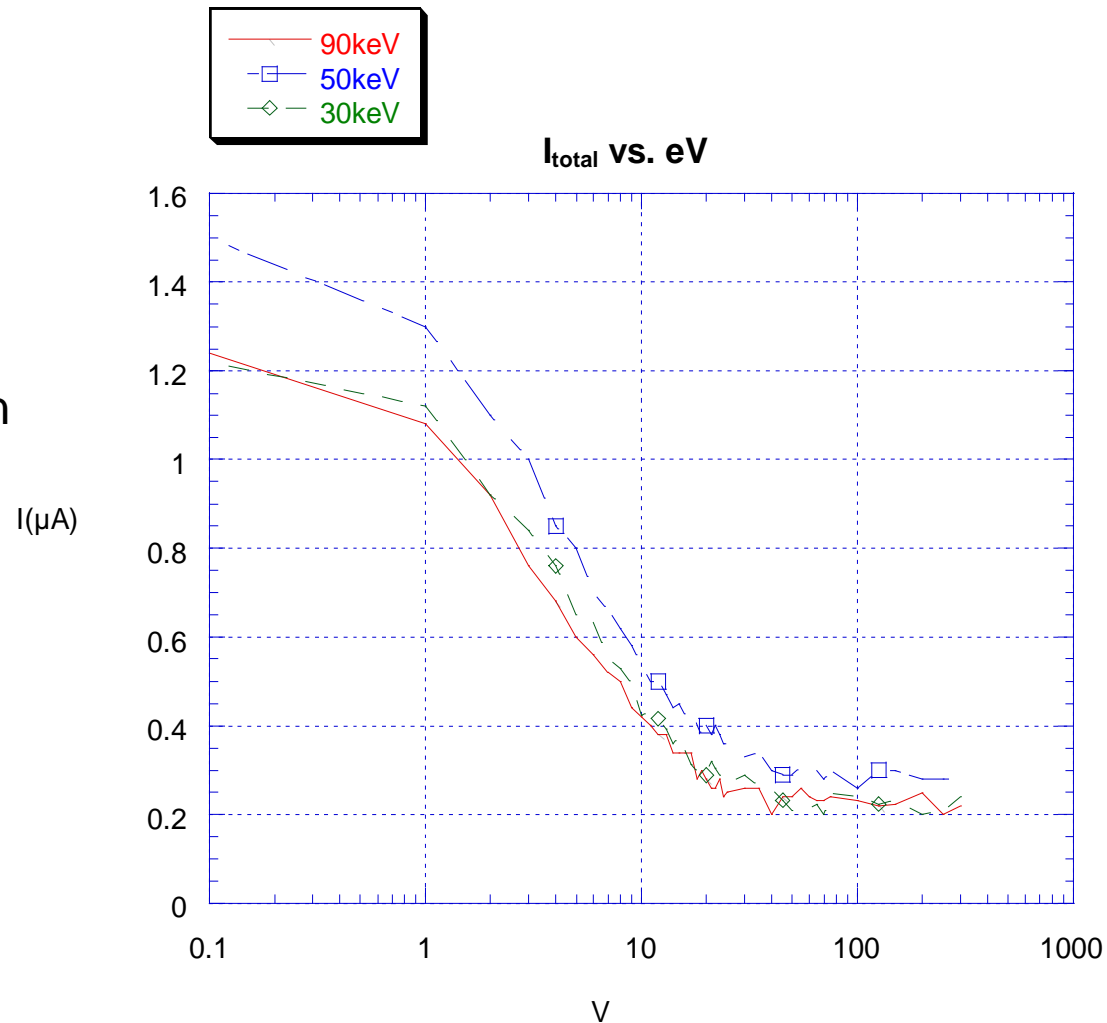



# Faraday Cup with water cooling **CAS**

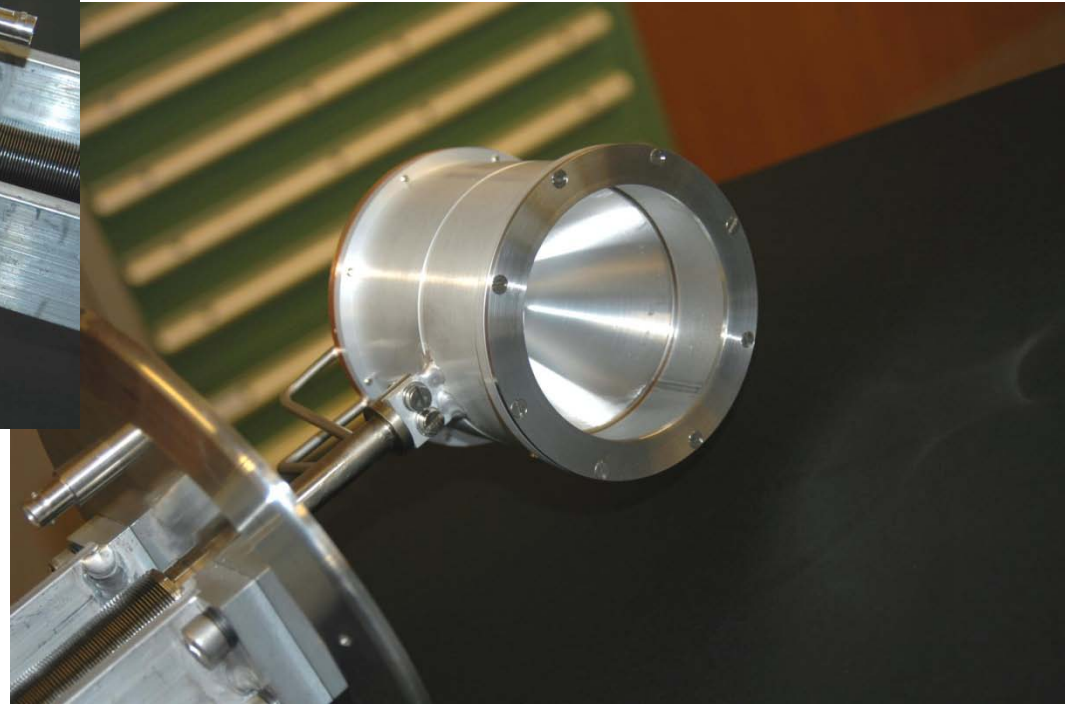


For higher intensities  
water cooling may be needed



# The Ideal Transformer

CAS

$$U(V) \equiv I_{beam} \frac{dI_{beam}}{dt} \frac{R}{N} e^{-\frac{t}{\tau_{drop}}}$$


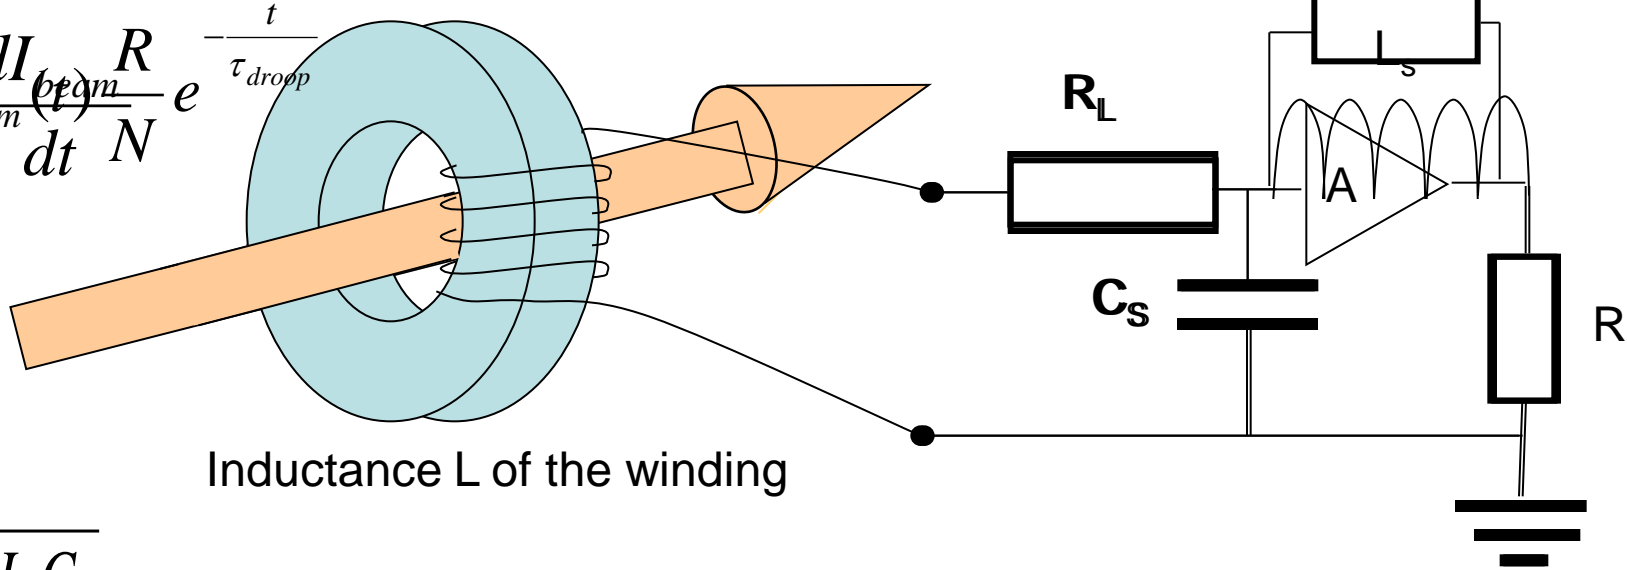



Inductance L of the winding

$$\tau_{rise} = \sqrt{L_s C_s}$$

$$\tau_{drop} = \frac{L}{R + R_L} \approx \frac{L}{R_L}$$

Transformer output signal

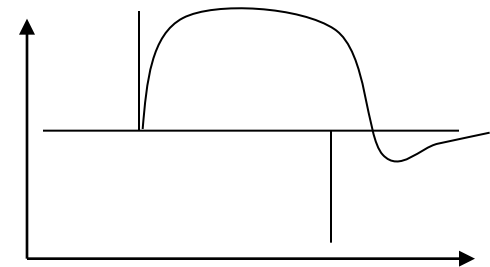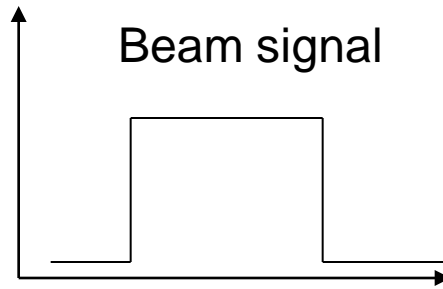

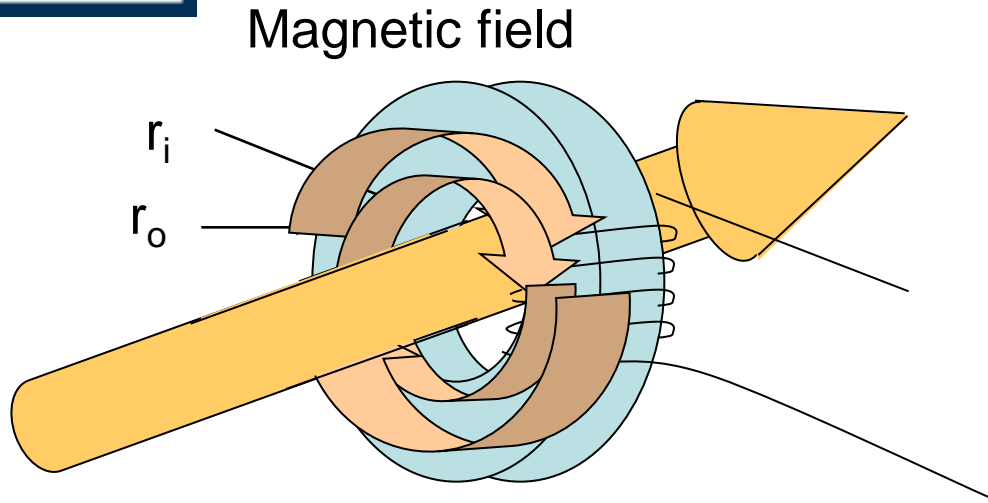

Fields are very low

Capture magnetic field lines with cores of high relative permeability

(CoFe based amorphous alloy Vitrvac:  $\mu_r = 10^5$ )

Beam current

$$I_{\text{beam}} = \frac{qeN}{t} = \frac{qeN\beta c}{l}$$


$$L = \frac{\mu_0 \mu_r}{2\pi} l N^2 \ln \frac{r_o}{r_i}$$





# Principle of a fast current transformer

# CAS

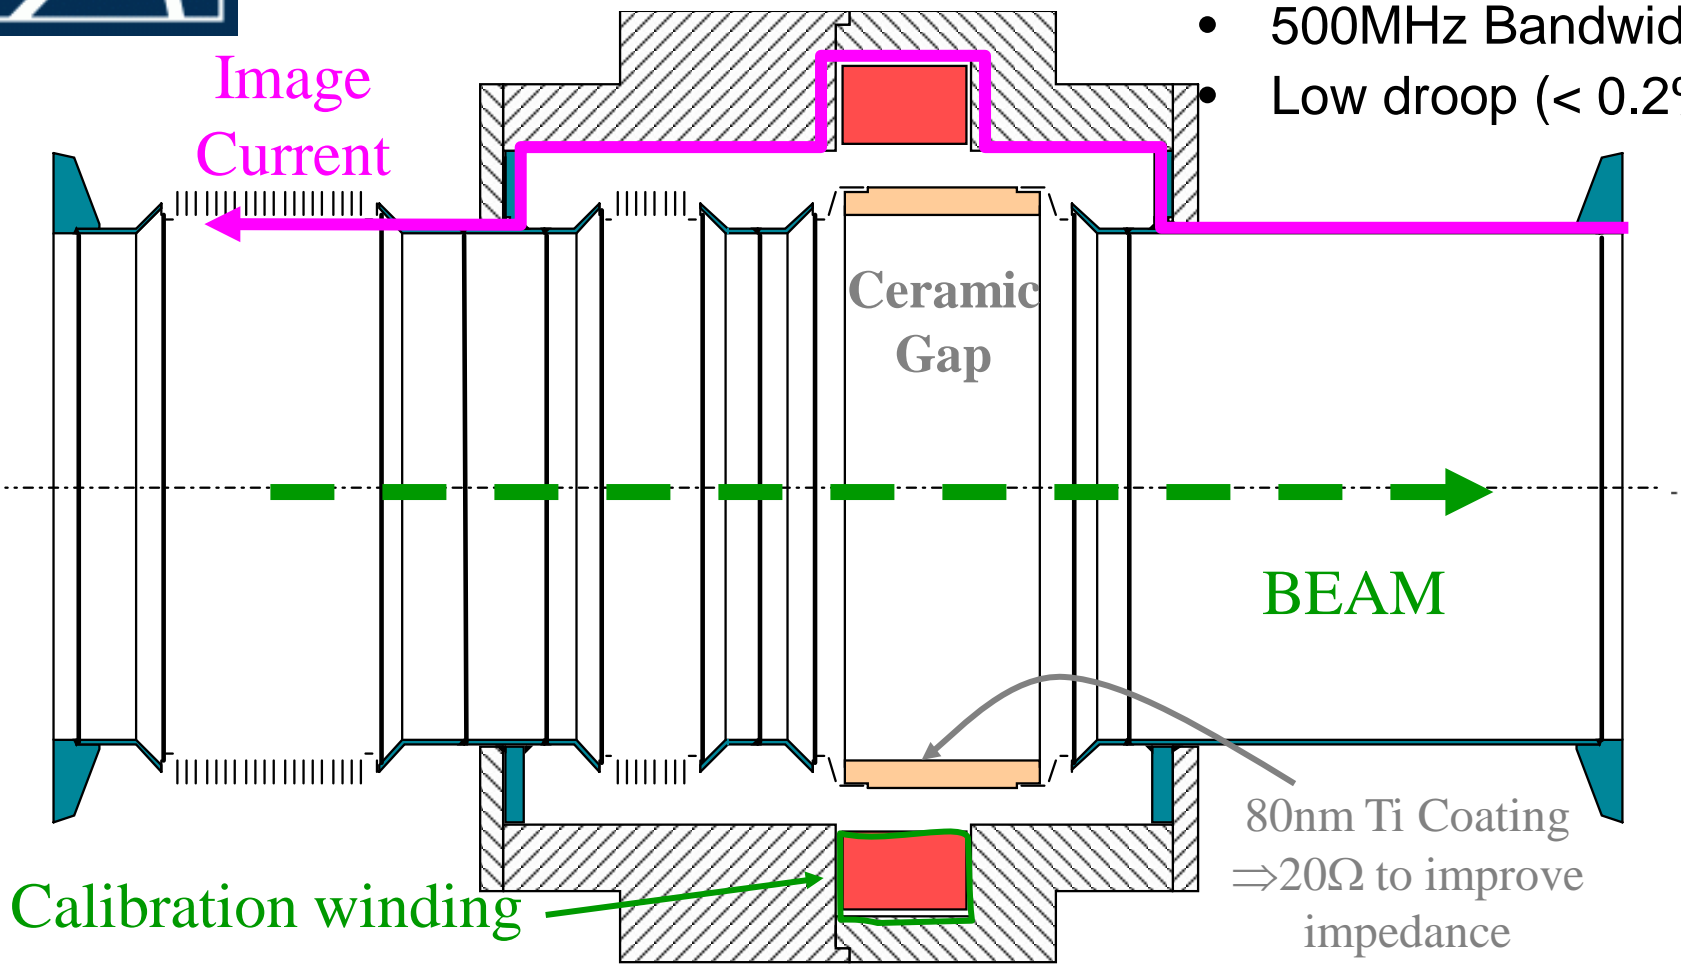


- 500MHz Bandwidth
- Low droop ( $< 0.2\%/μs$ )

80nm Ti Coating  
 $\Rightarrow 20\Omega$  to improve impedance



# Fast current transformers for the LHC

CAS


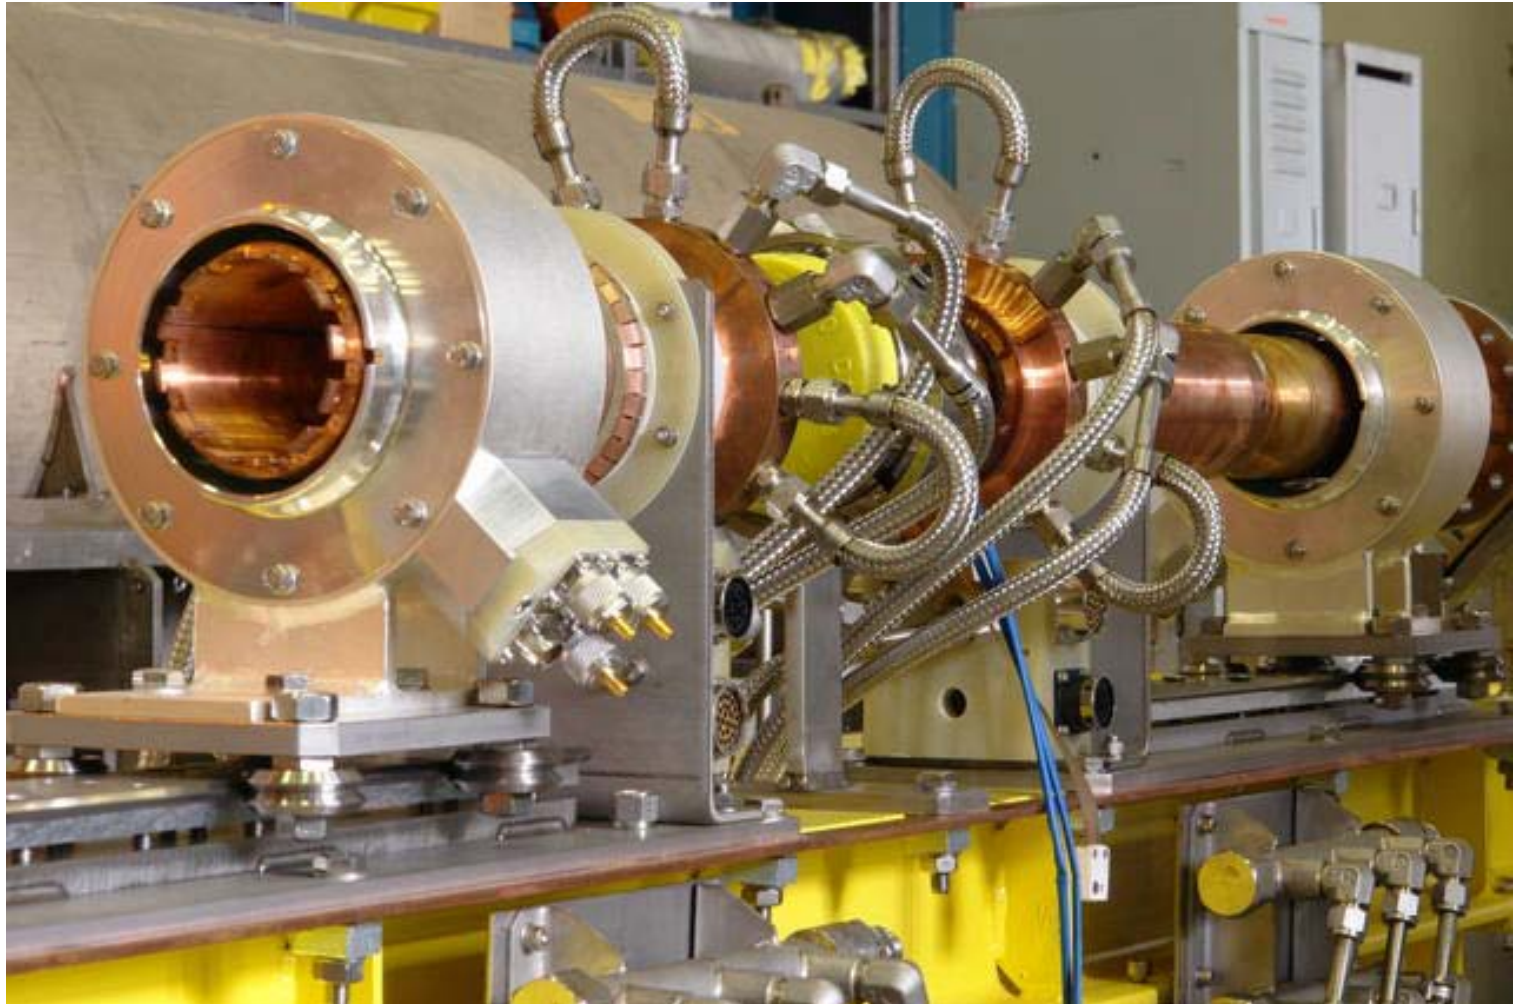




# Magnetic shielding


CAS

- Shield should extend along the vacuum chamber length  $>$  diameter of opening
- Shield should be symmetrical to the beam axis
- Air gaps must be avoided especially along the beam axis
- Shield should have highest  $\mu$  possible but should not saturate

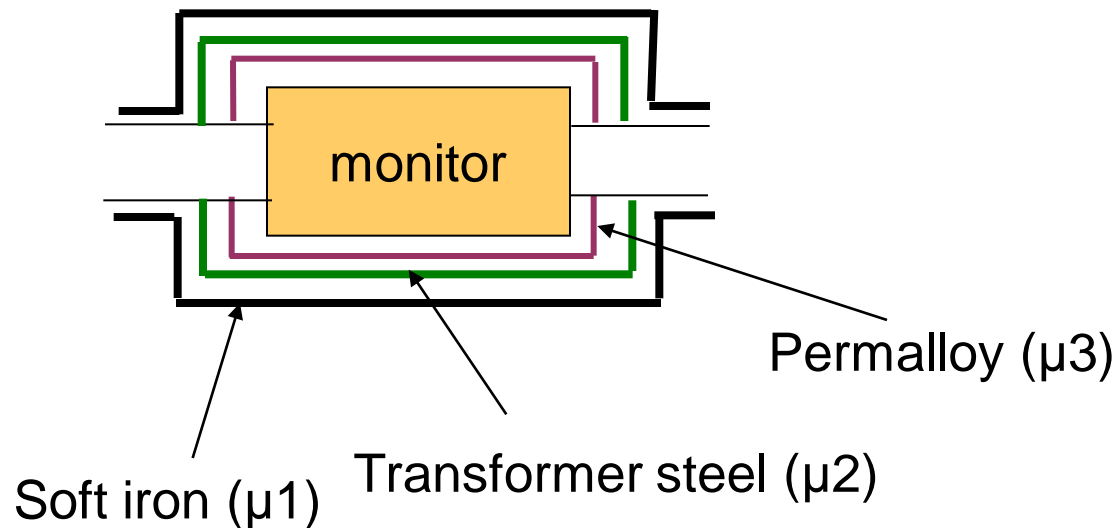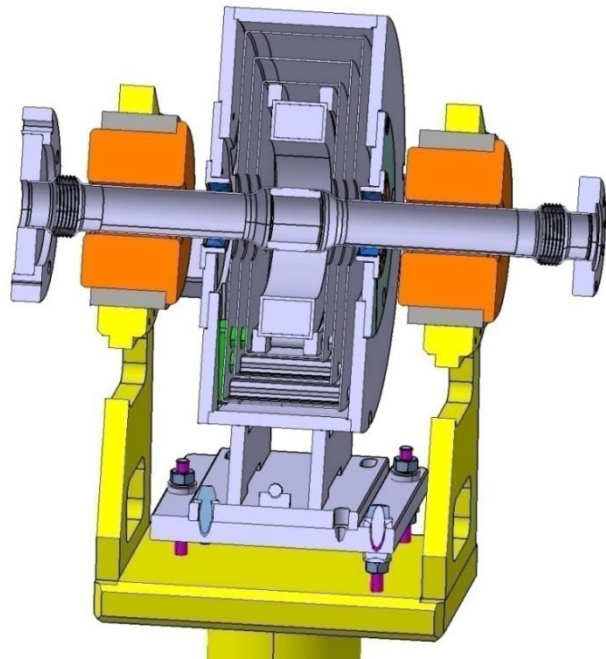



# Calibration of AC current transformers **CAS**

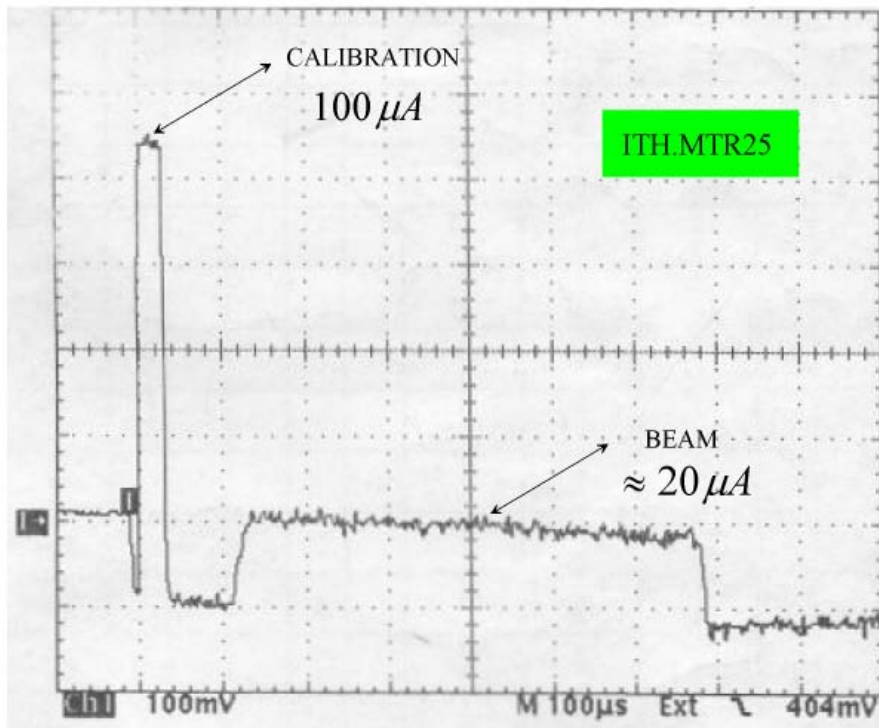


- The transformer is calibrated with a very precise current source
- The calibration signal is injected into a separate calibration winding
- A calibration procedure executed before the running period
- A calibration pulse before the beam pulse measured with the beam signal





# Current transformer and electronics

CAS

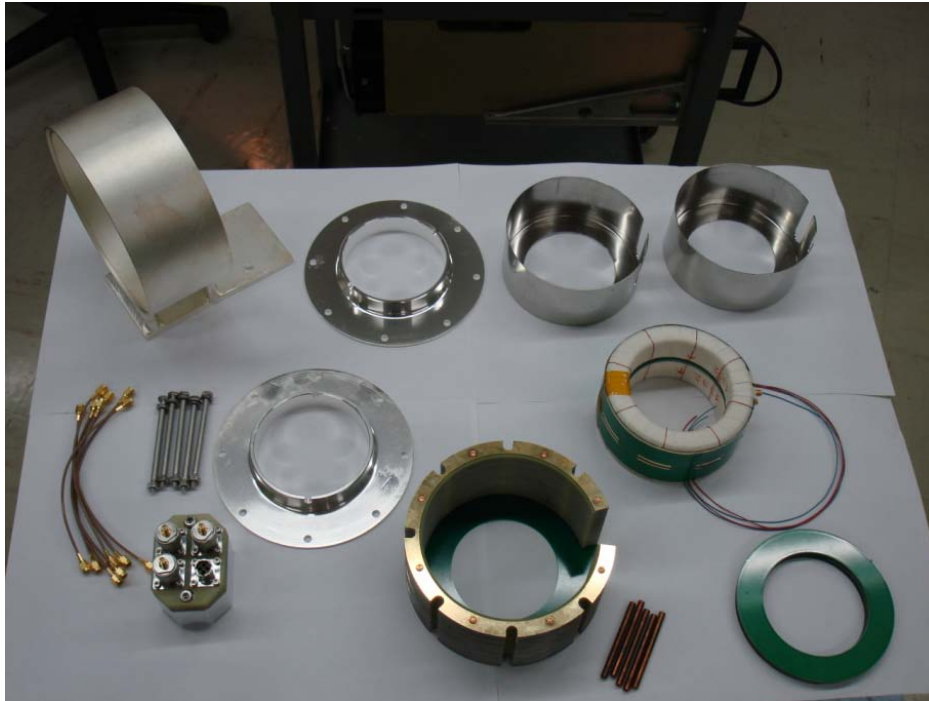






# Display of transformer readings

# CAS

- First result from LHC FBCT
- Measurement of bunch intensity
- Diminishing intensity due to debunching
- Beam losses will trigger machine protection system

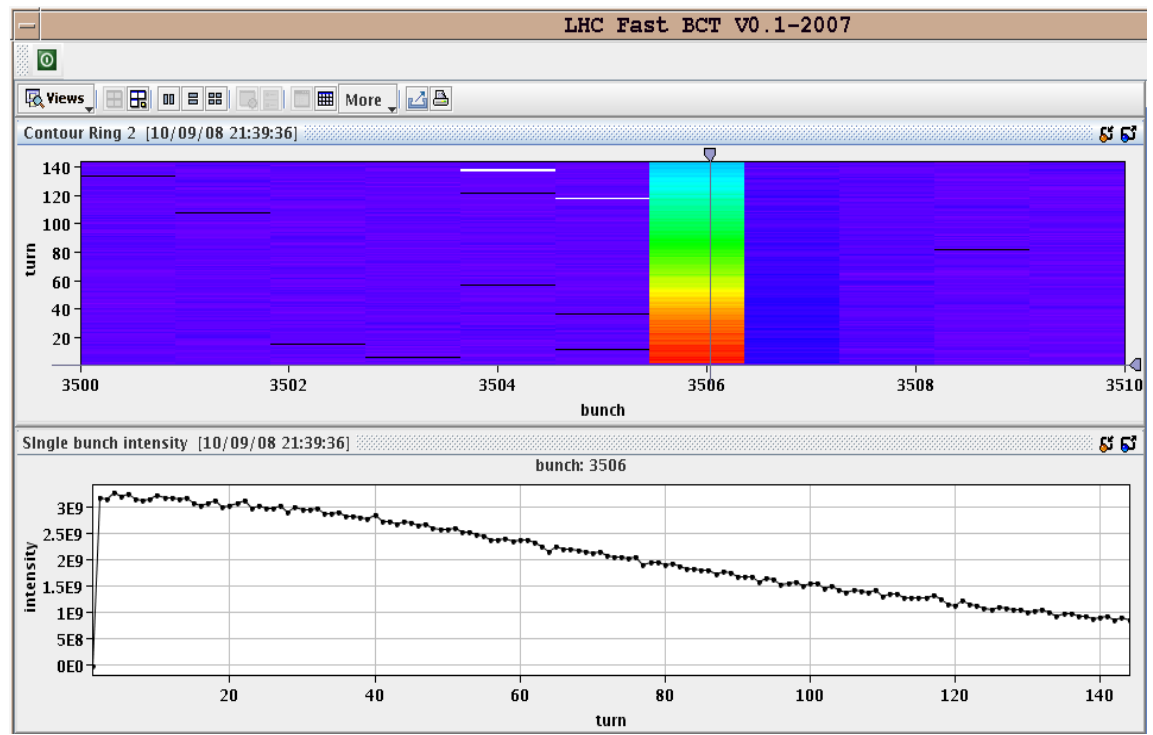




# The DC current transformer

CAS


- AC current transformer can be extended to very long droop times but not to DC
- Measuring DC currents is needed in storage rings
- Must provide a modulation frequency
- Takes advantage of non/linear magnetisation curve

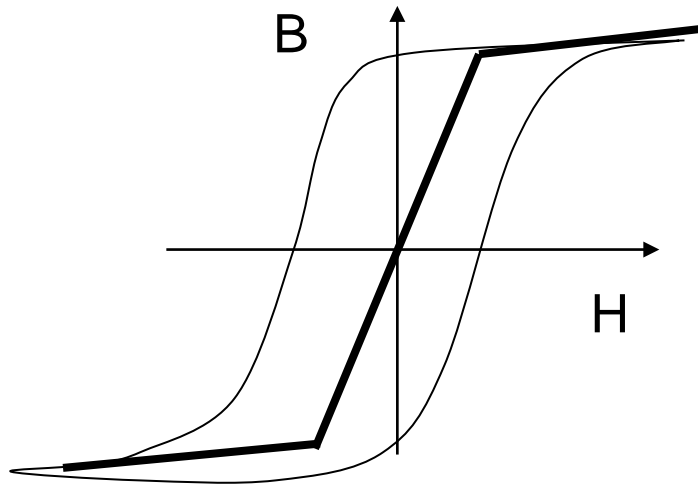




# Principle of DCCT

CAS

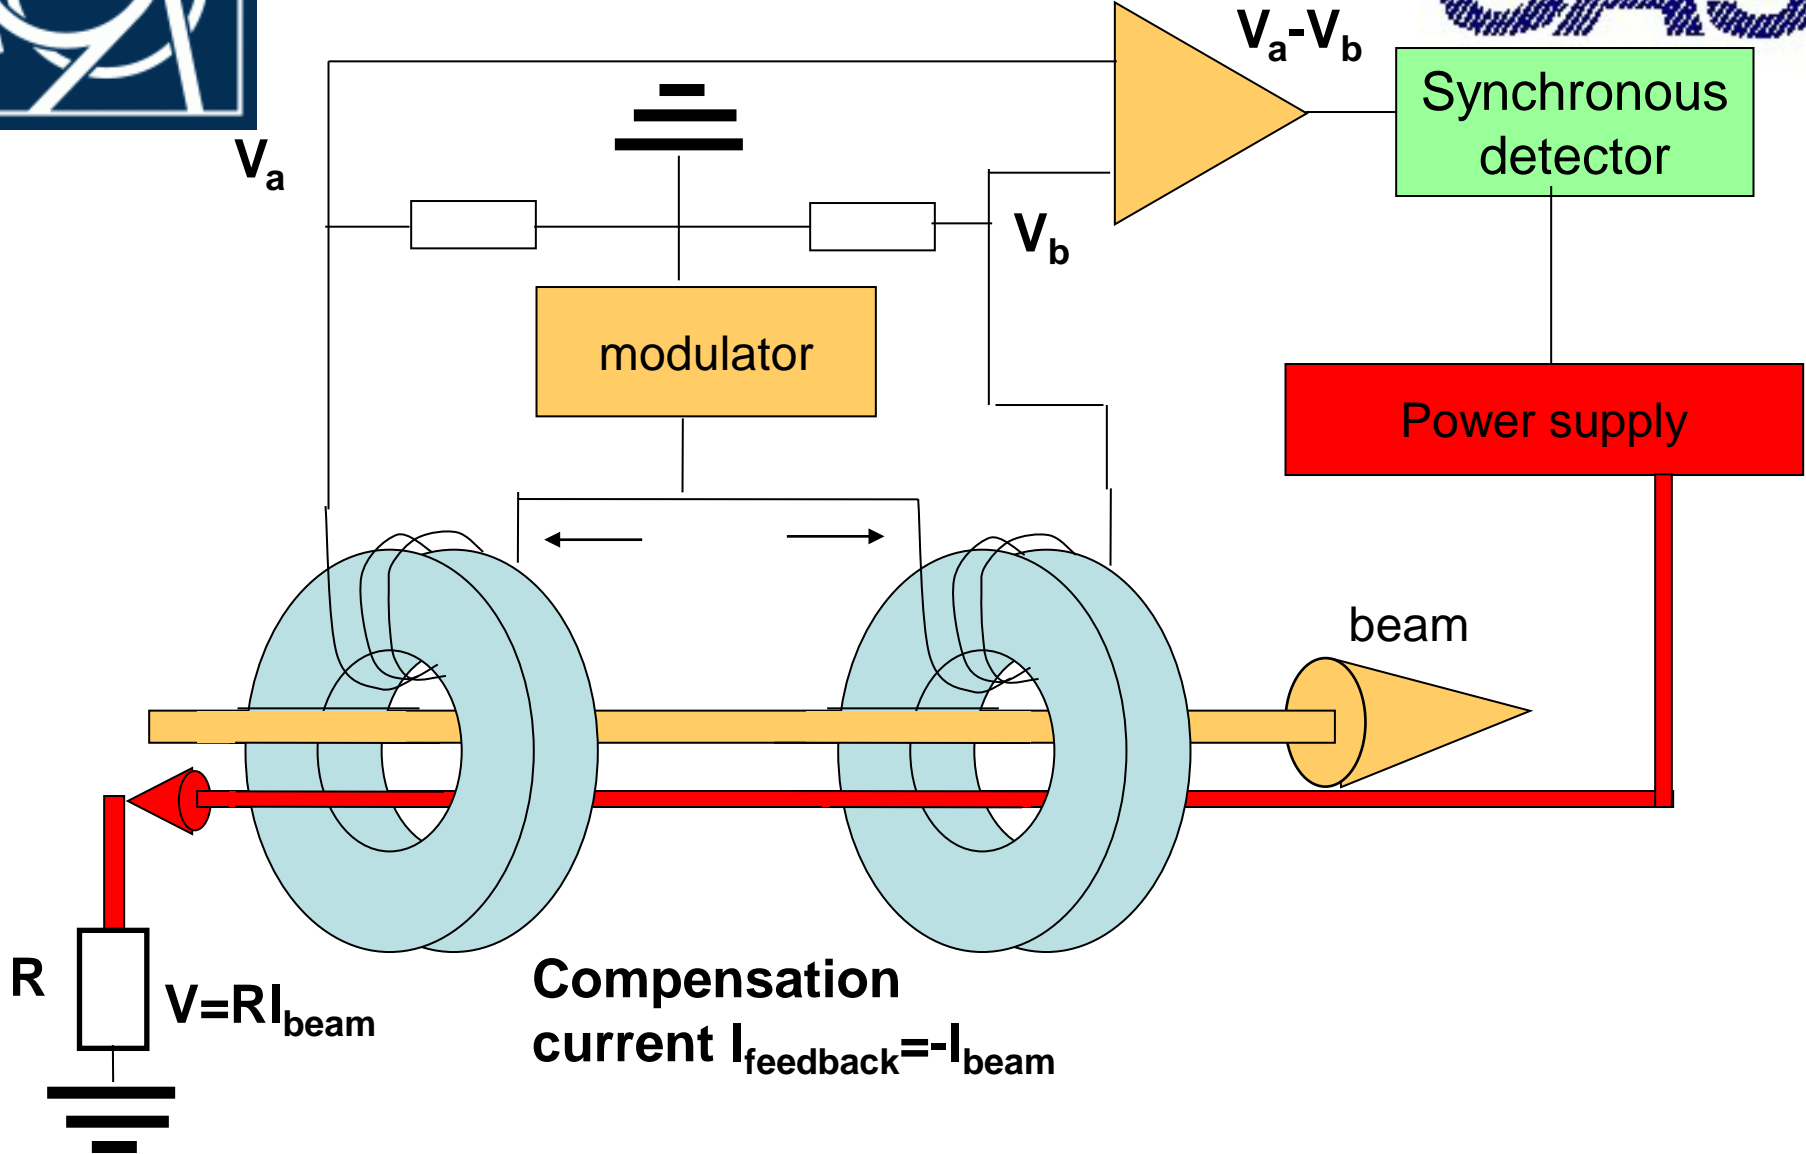



# Modulation of a DCCT without beam

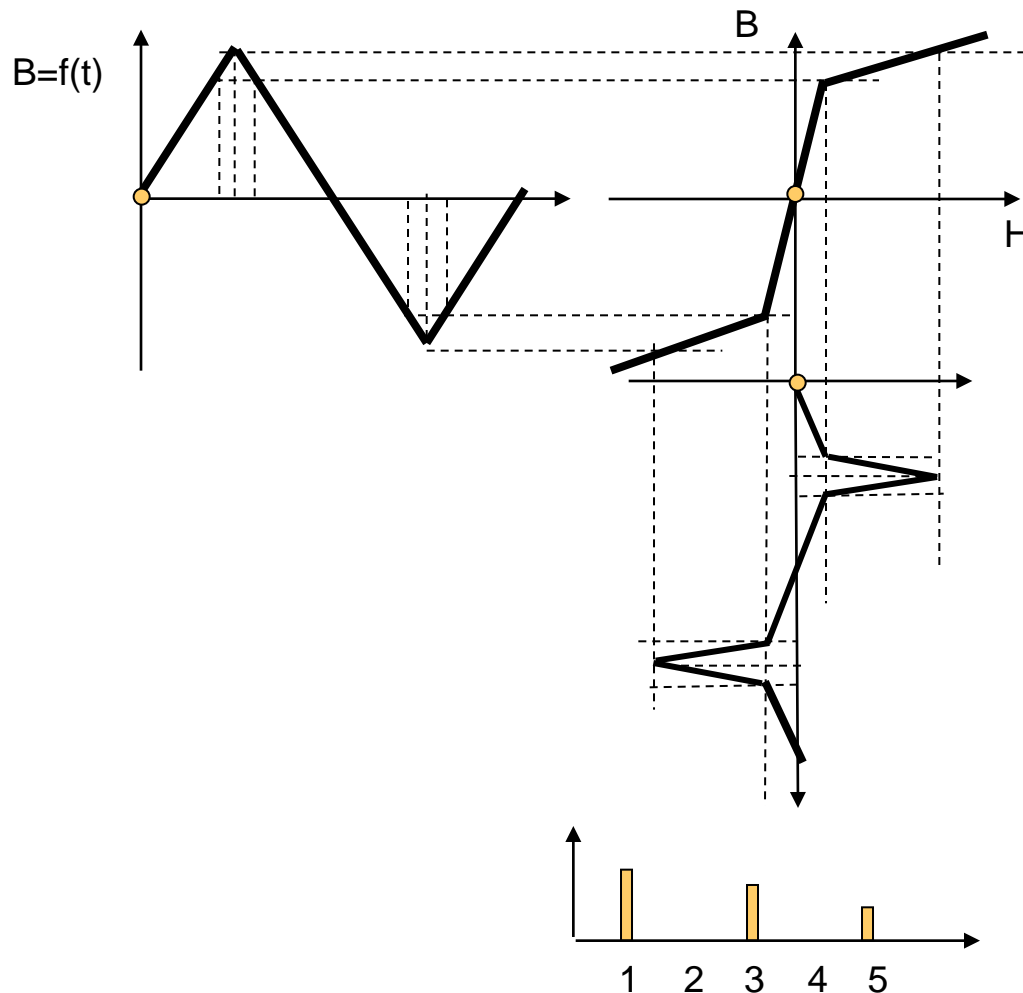

$$U = NA \frac{dB}{dt}$$


$$B = \frac{\int U dt}{NA} + B_0$$

Modulation current has only odd harmonic frequencies since the signal is symmetric



# Modulation of a DCCT with beam

CAS

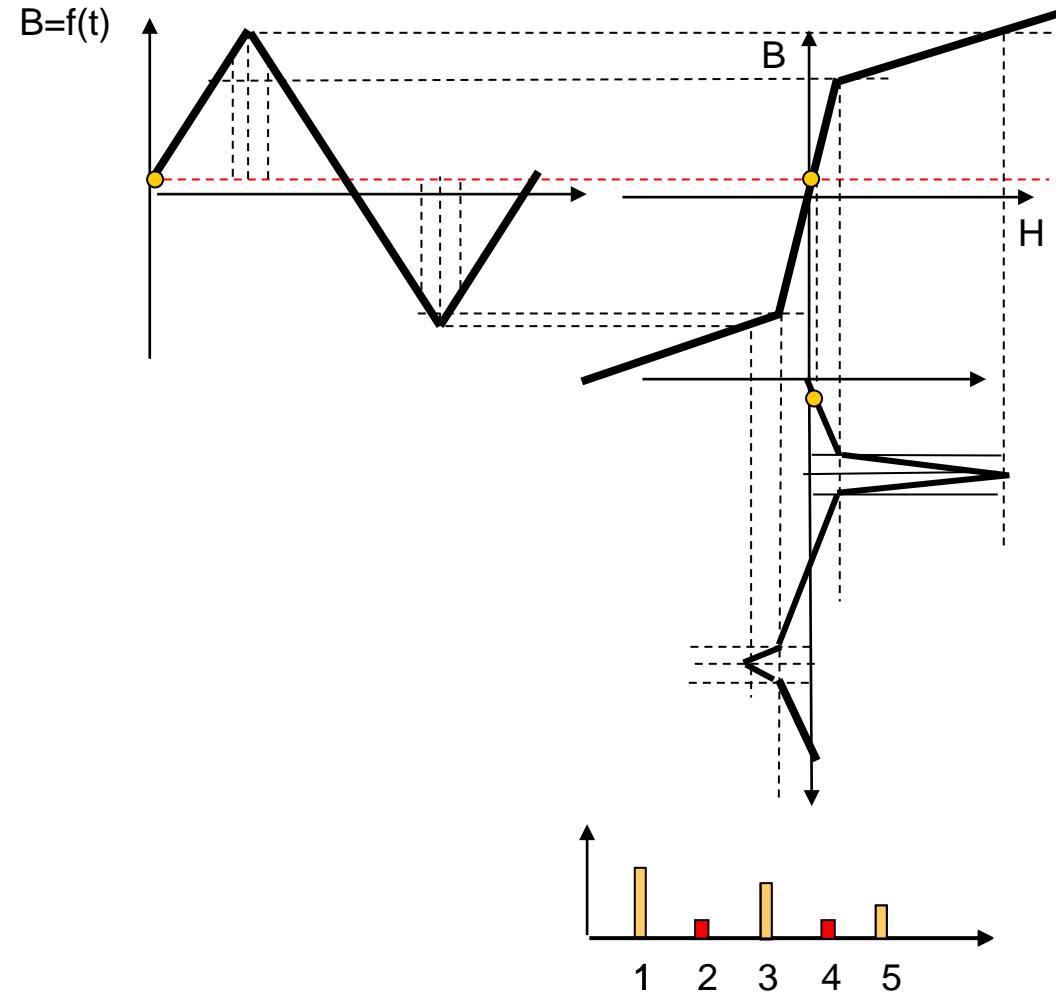

Sum signal becomes non-zero  
Even harmonics appear






## Modulation current difference signal with beam

CAS

- Difference signal has  $2\omega_m$
- $\omega_m$  typically 200 Hz – 10 kHz
- Use low pass filter with  $\omega_c \ll \omega_m$
- Provide a 3rd core, normal AC transformer to extend to higher frequencies

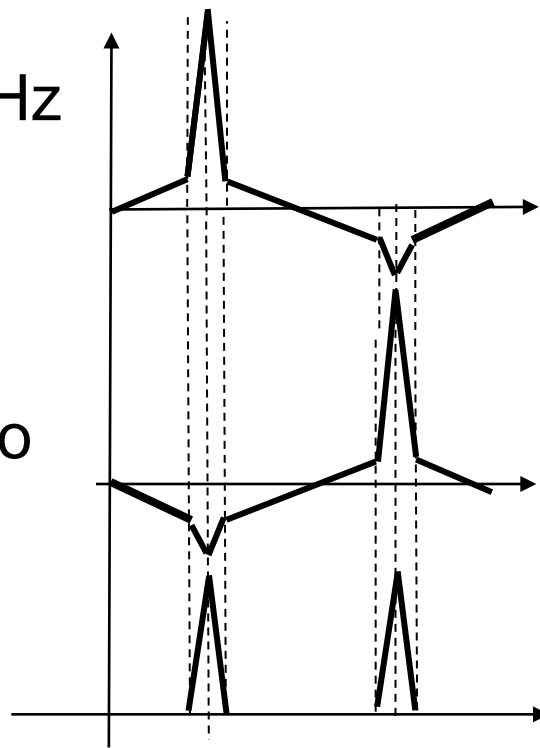



# Photo of DCCT internals

CAS






# Results from DCCT



Beam 2  
DCCT sees first  
circulating beam


Injections into LHC

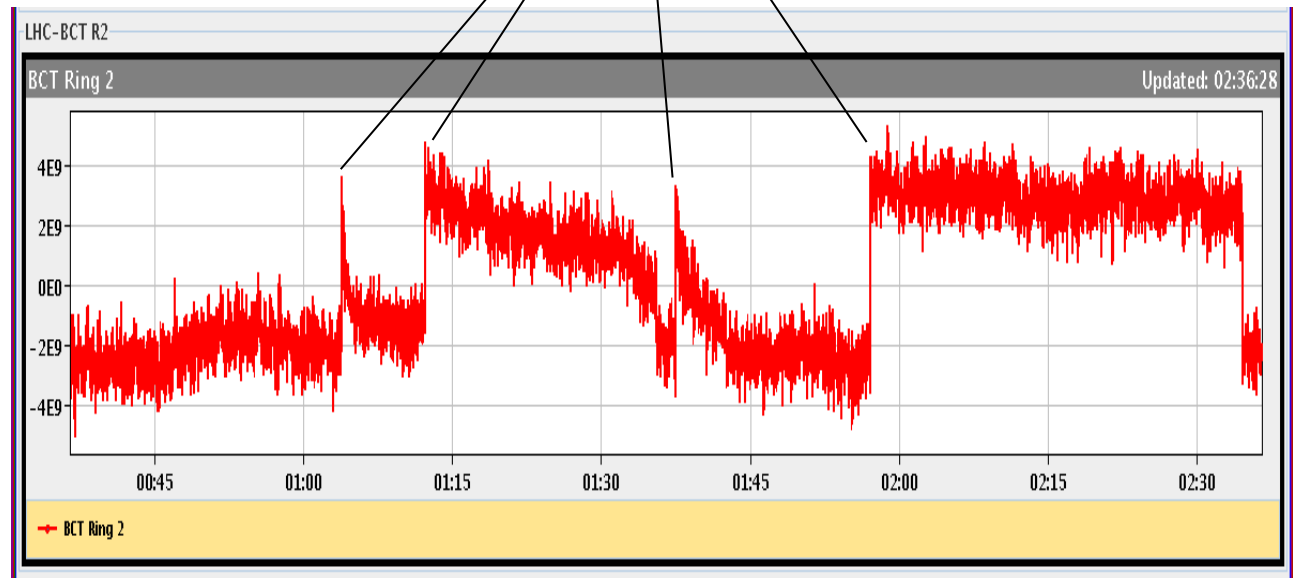



# Measuring Beam Position – The Principle


CAS

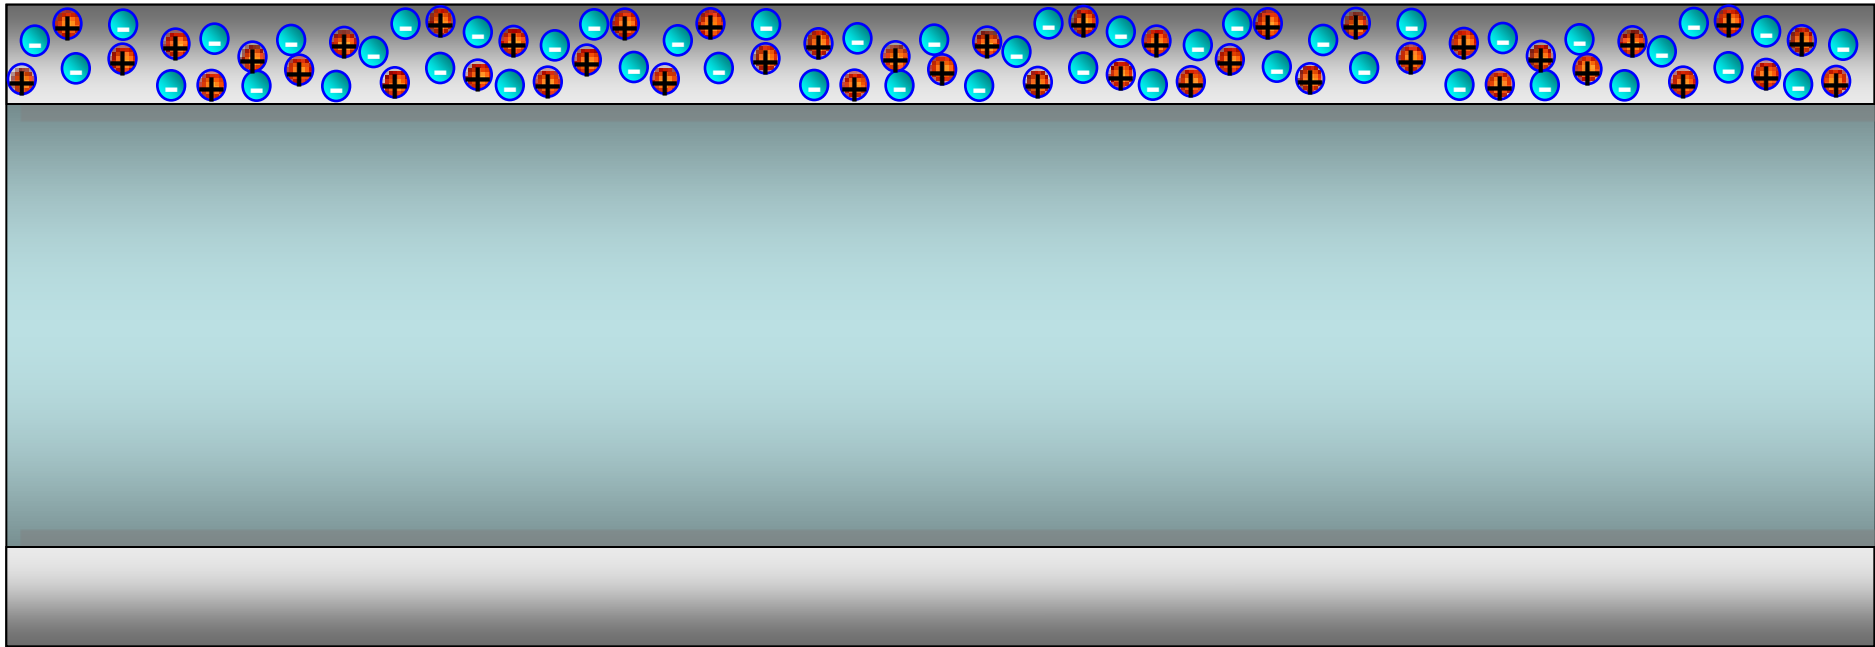



# Wall Current Monitor – The Principle

CAS



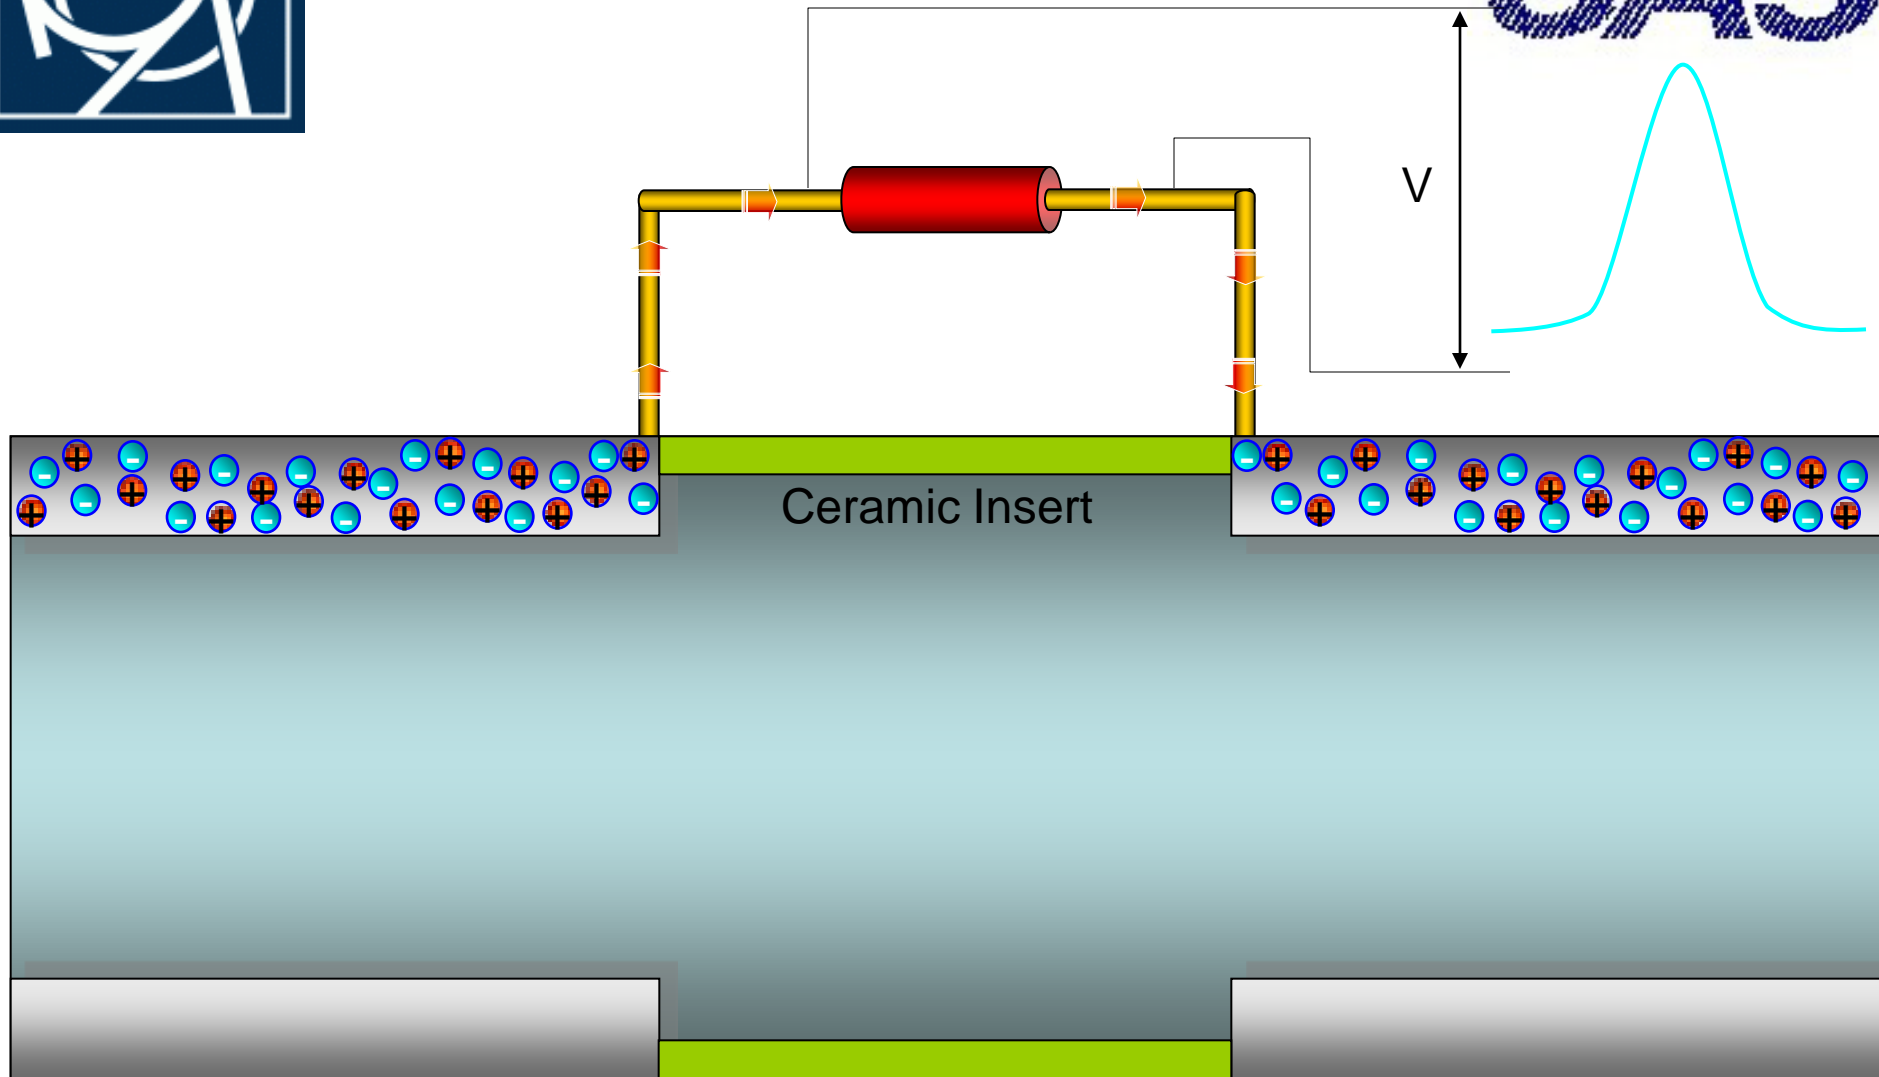






# Wall Current Monitor – Beam Response


CAS

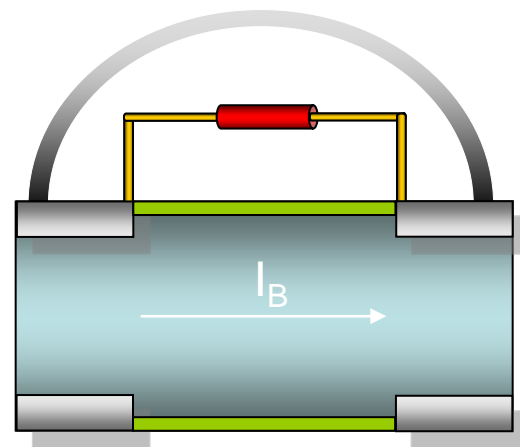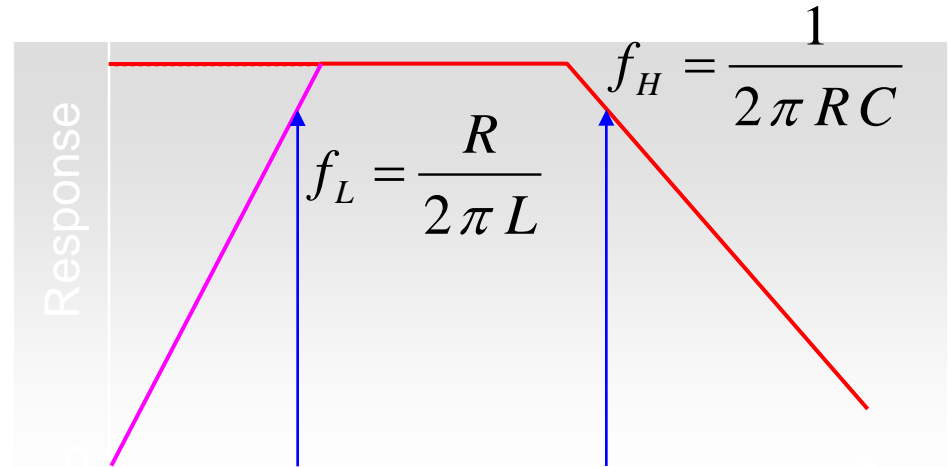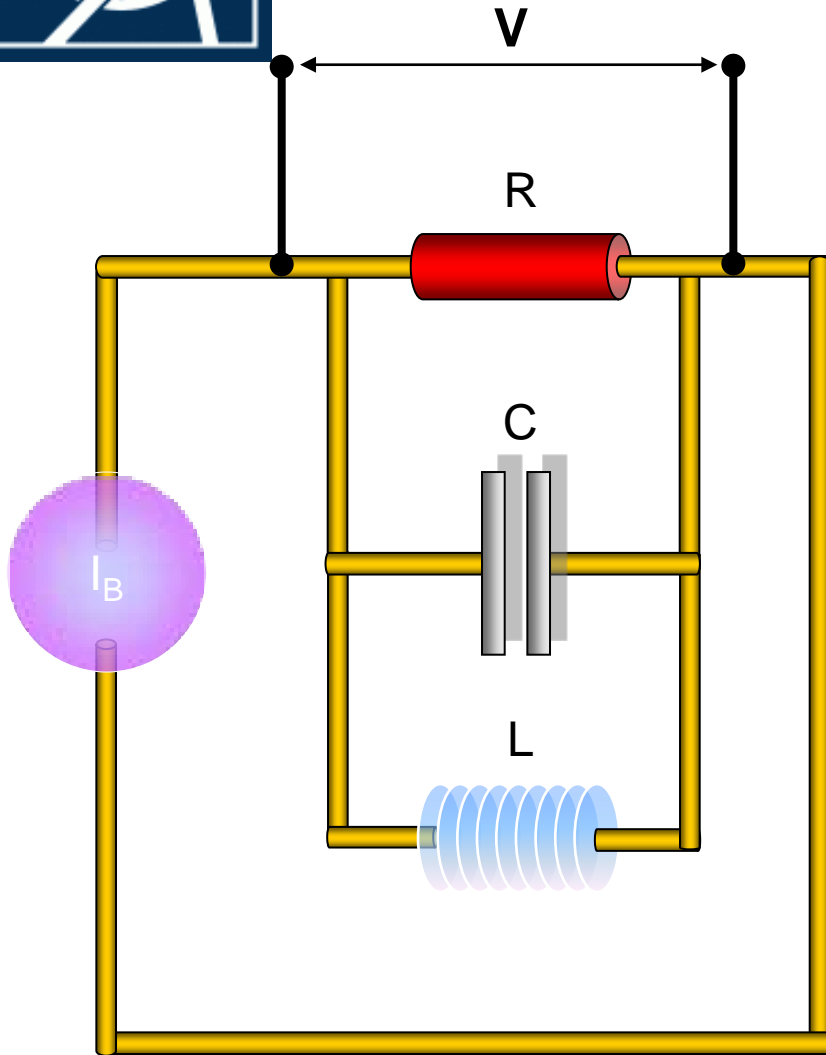



# Electrostatic Monitor – The Principle




CAS

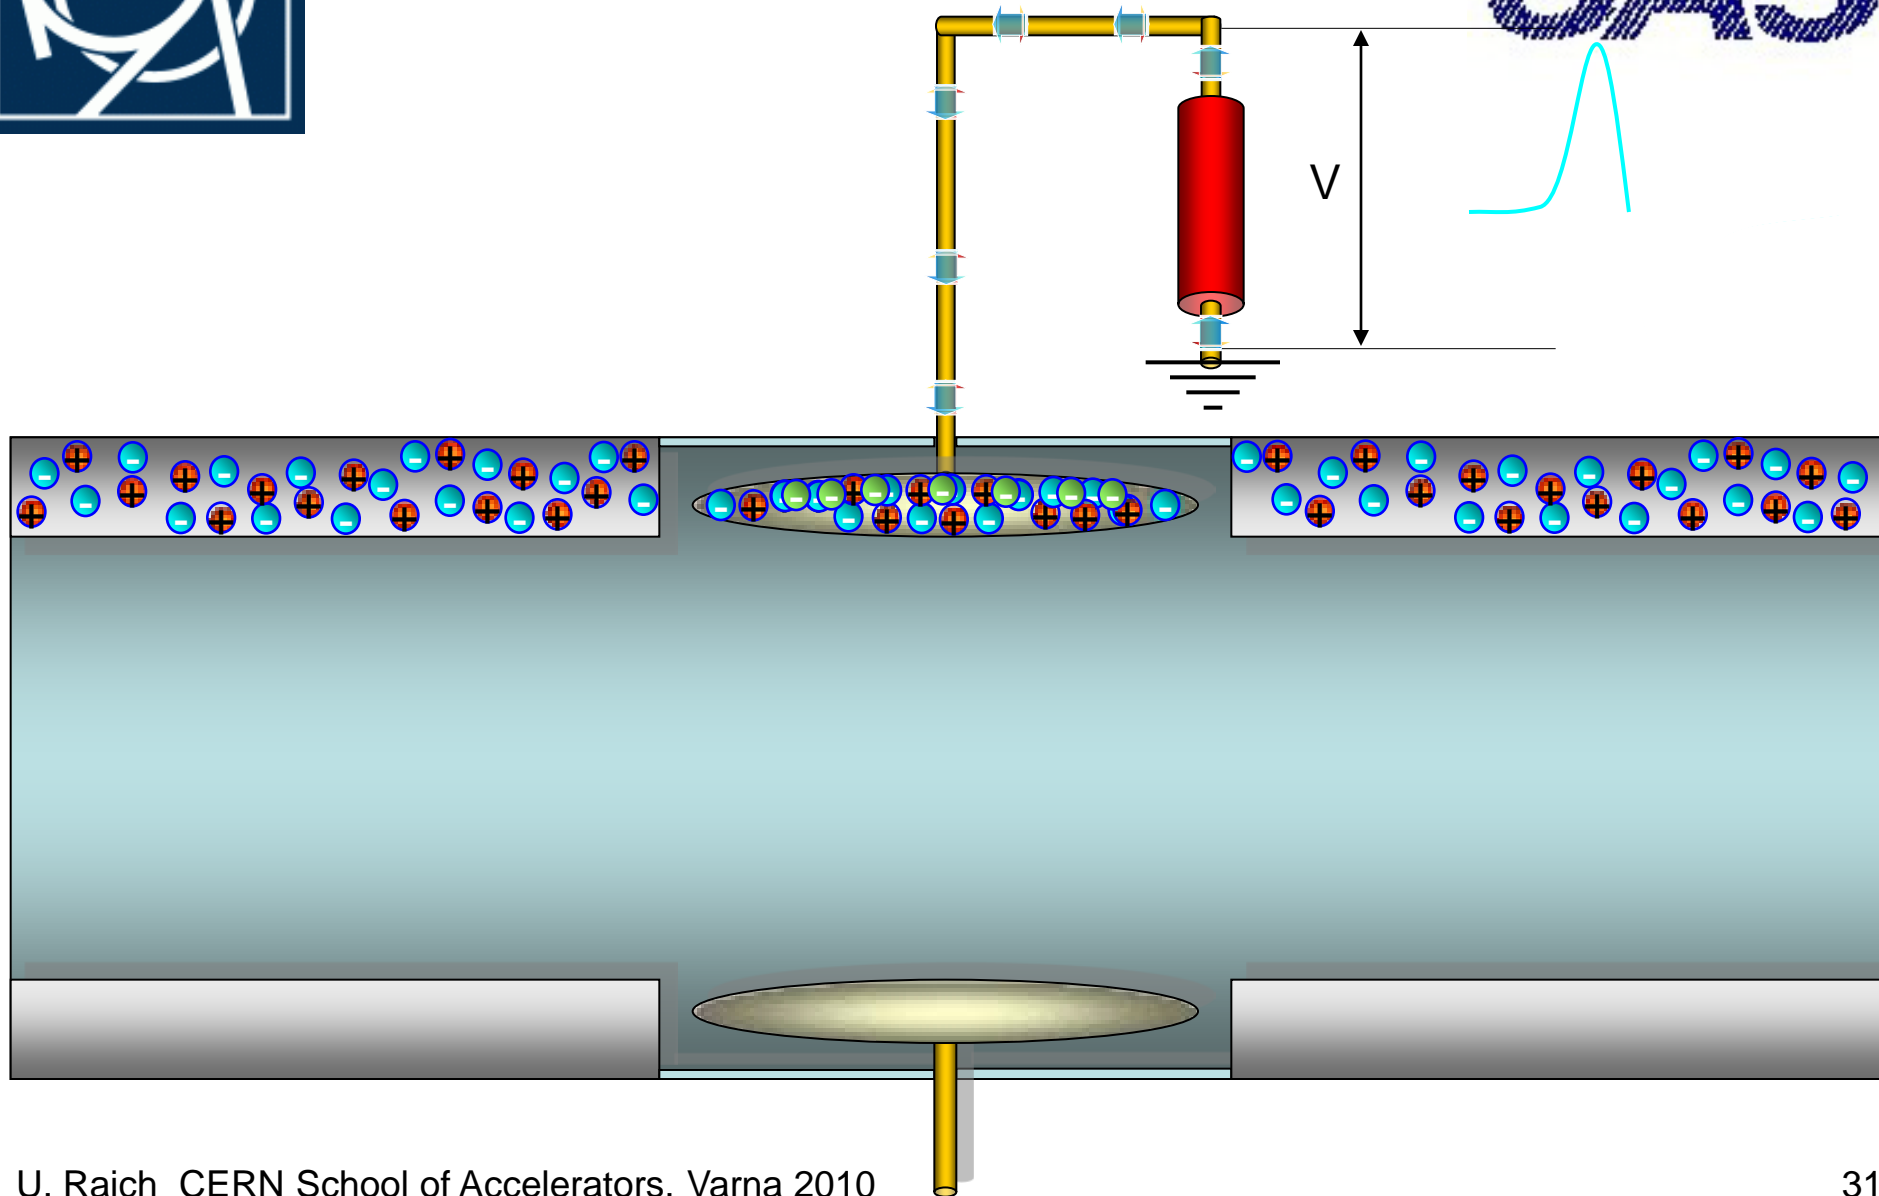



# Electrostatic Monitor – Beam Response


CAS

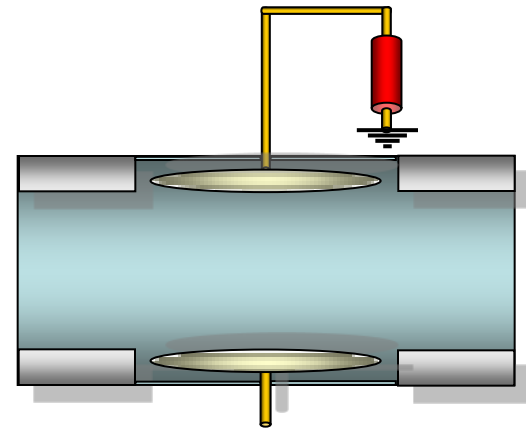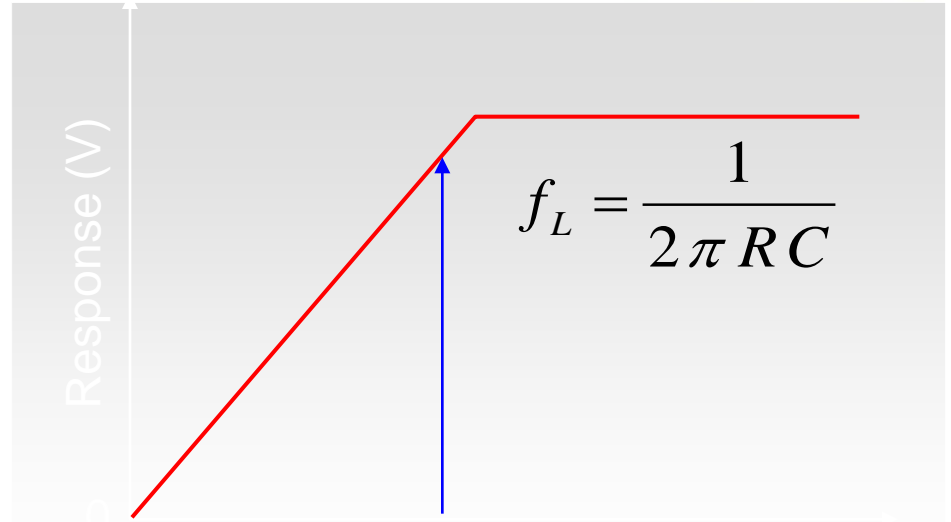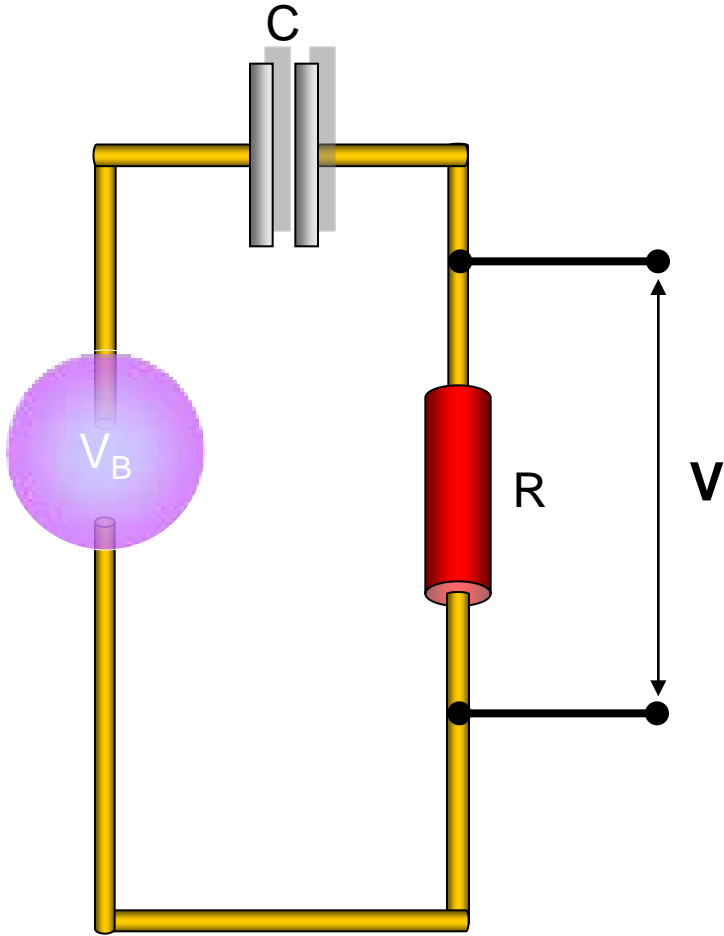



# Position measurements

CAS

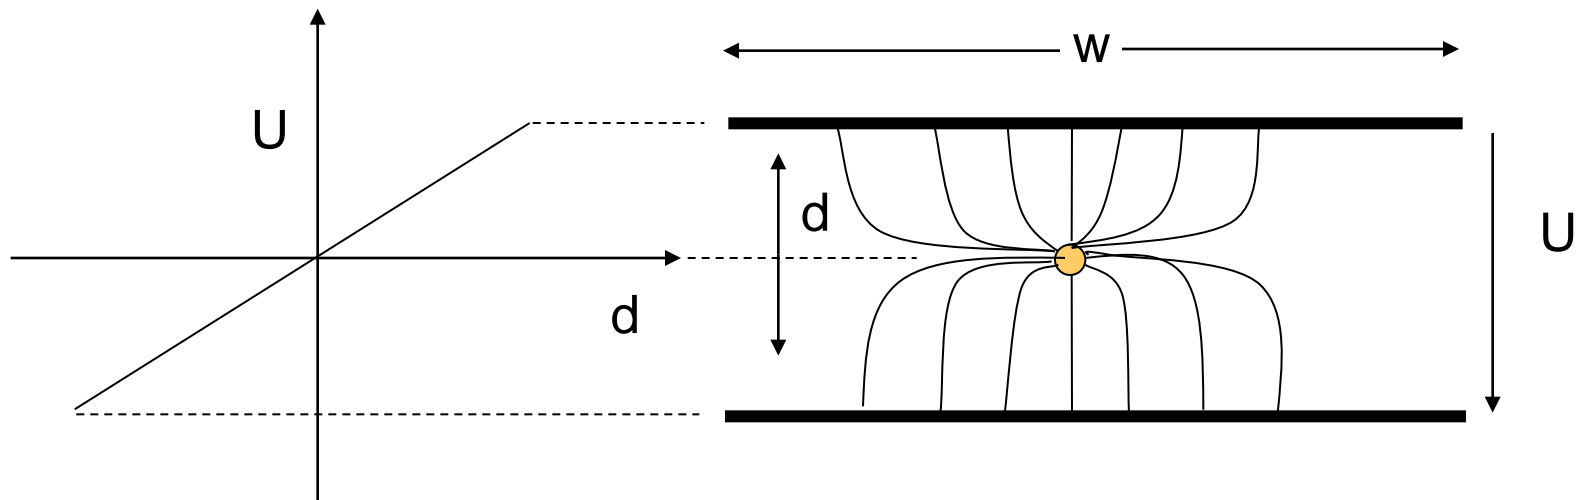


If the beam is much smaller than  $w$ , all field lines are captured and  $U$  is a linear function with replacement  
else: Linear cut (projection to measurement plane must be linear)




# Shoebox pick-up

CAS

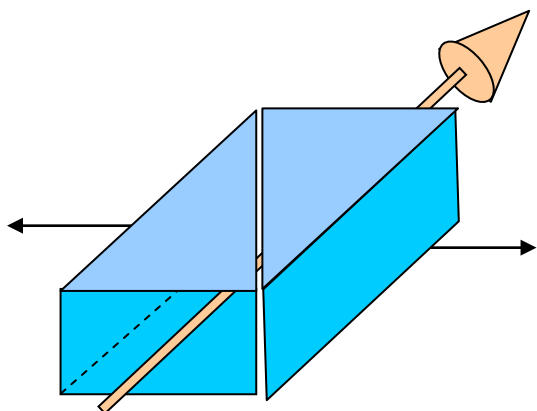

Linear cut through a shoebox

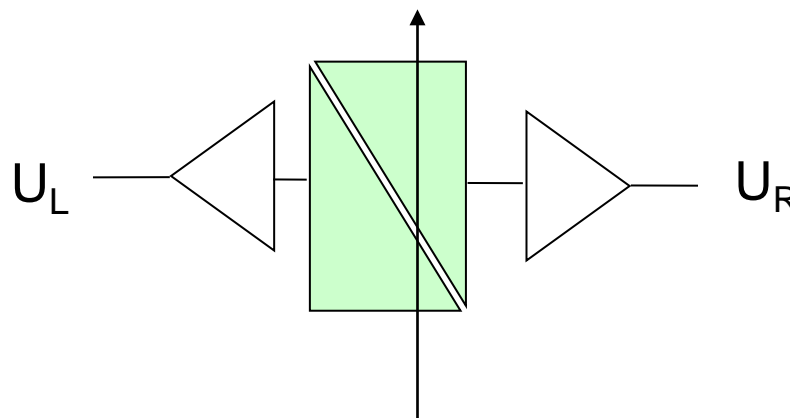


$$X \propto \frac{U_L - U_R}{U_L + U_R} = \frac{\Delta}{\Sigma}$$



# Doubly cut shoebox

- Can measure horizontal and vertical position at once
- Has 4 electrodes

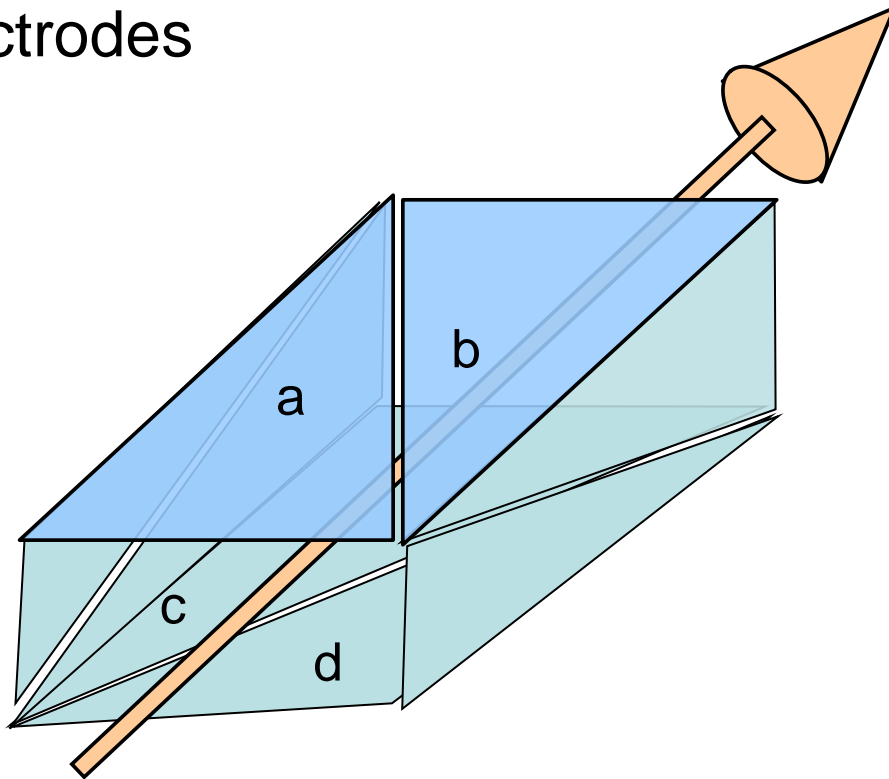




# Simultaneous horizontal and vertical measurement


CAS

horizontal

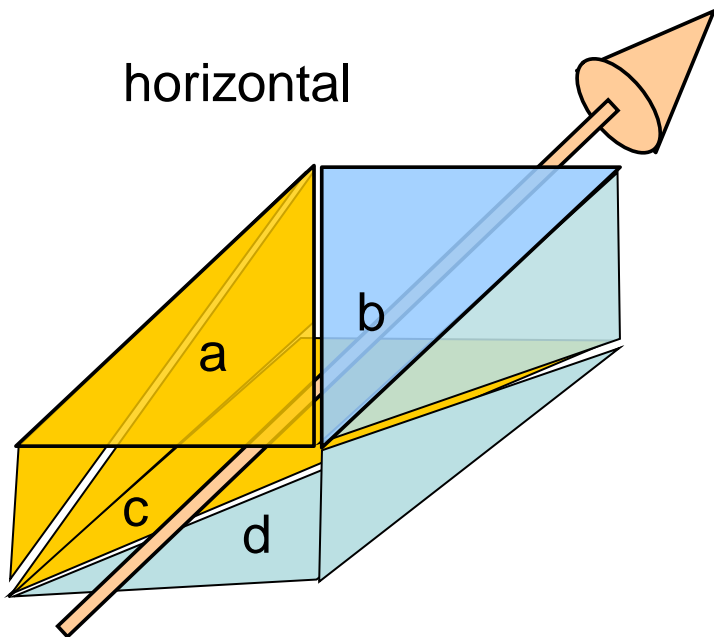

$$X = \frac{(U_a + U_c) - (U_b + U_d)}{\Sigma U}$$

vertical

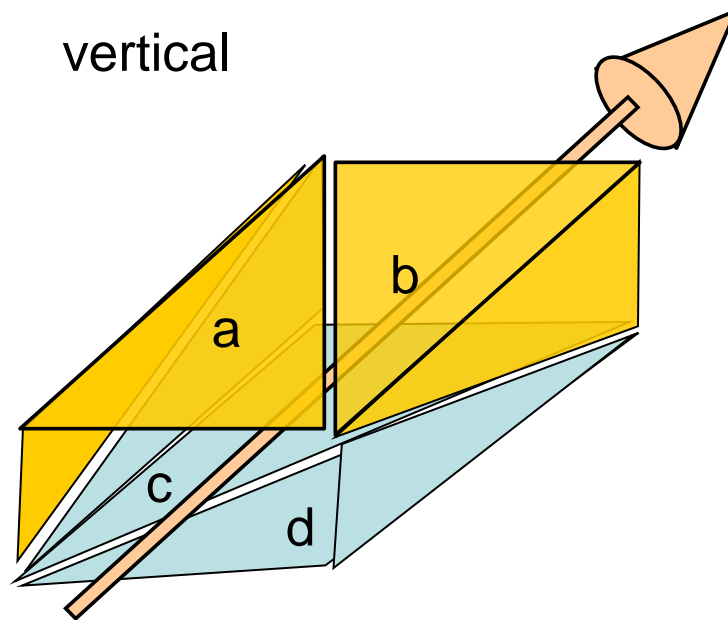


$$Y = \frac{(U_a + U_b) - (U_c + U_d)}{\Sigma U}$$



# Interaction of particles with matter

CAS

- Coulomb interaction
- Average force in s-direction=0
- Average force in transverse direction  $\langle \rangle 0$
- Mostly large impact parameter  $\Rightarrow$  low energy of ejected electron
- Electron mostly ejection transversely to the particle motion

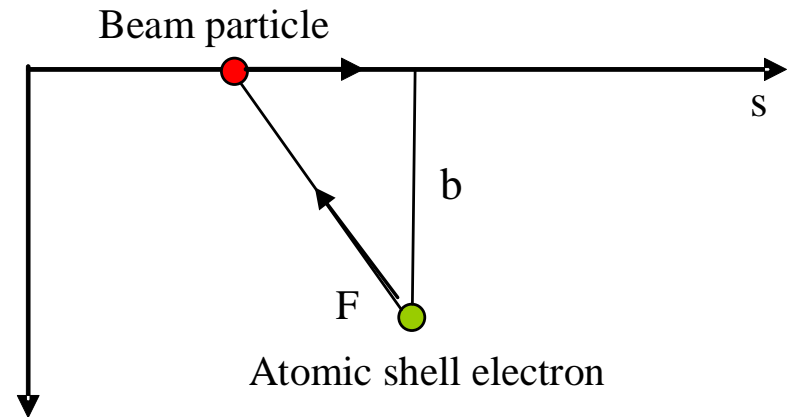



# Bethe Bloch formula

CAS

$$-\frac{dE}{dx} = 4\pi N_A r_e^2 m_e c^2 \frac{Z_T}{A_T} \rho \frac{Z_p^2}{\beta^2} \left[ \ln \frac{2m_e c^2 \gamma^2 \beta^2}{I} - \beta^2 \right]$$


- with the following constants:
  - $N_A$ : Avogadro's number
  - $m_e$  and  $r_e$ : electron rest mass and classical electron radius
  - $c$ : speed of light
- the following target material properties:
  - $\rho$ : material density
  - $A_T$  and  $Z_T$ : the atomic mass and nuclear charge
- and the particle properties:
  - $Z_p$ : particle charge
  - $\beta$ : the particles velocity and  $\gamma = \sqrt{1 - \beta^2}$

Dependance on  $Z_p^2$



# High energy loss a low energies

CAS

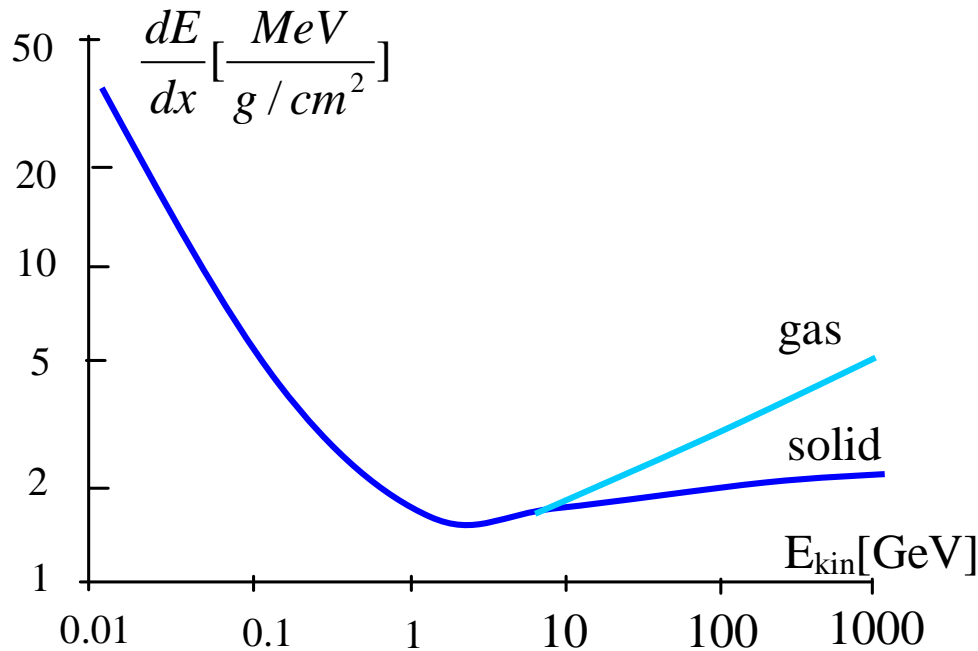

Heavy ions at low energy are stopped within a few micro-meters  
All energy is deposited in a very small volume





# Scintillating Screens

CAS

Method already applied in cosmic ray experiments


- Very simple
- Very convincing

Needed:

- Scintillating Material
- TV camera
- In/out mechanism

Problems:

- Radiation resistance of TV camera
- Heating of screen (absorption of beam energy)
- Evacuation of electric charges

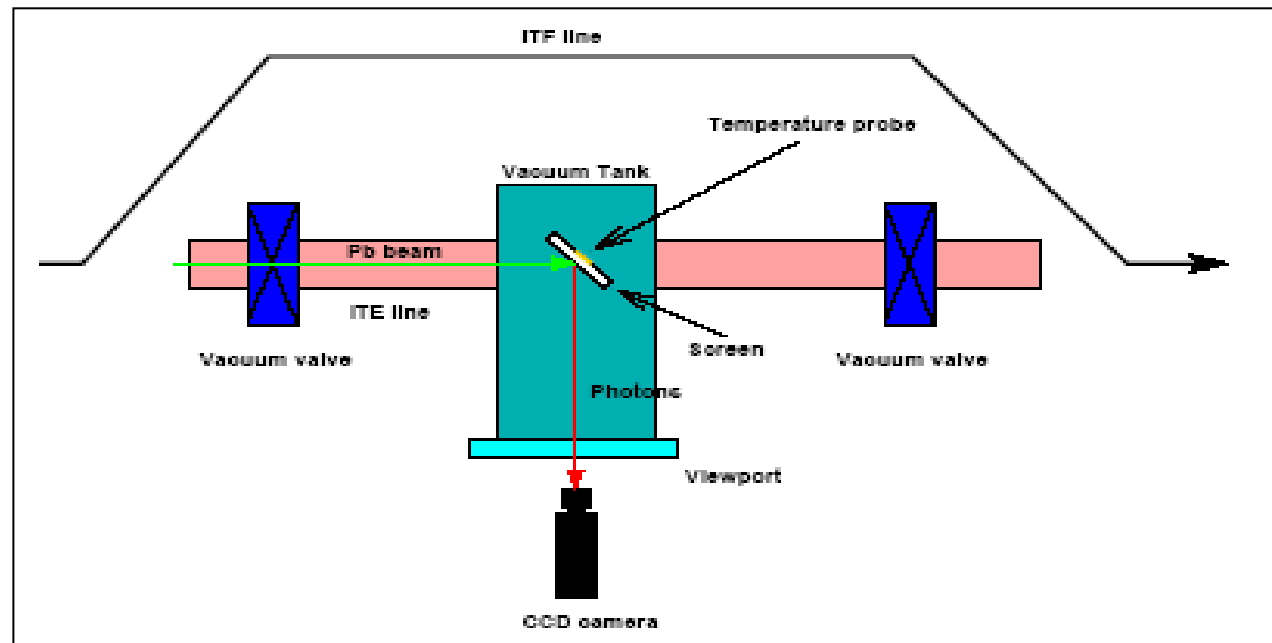



# Test for resistance against heat-shock





Material	$\rho$ g/cm <sup>3</sup>	$c_p$ at 20°C J/gK	$k$ at 100°C W/mK	$T_{max}$ °C	$R$ at 400 °C Ω.cm
Al <sub>2</sub> O <sub>3</sub>	3.9	0.9	30	1600	10 <sup>12</sup>
ZrO <sub>2</sub>	6	0.4	2	1200	10 <sup>3</sup>
BN	2	1.6	35	2400	10 <sup>14</sup>

Commonly used in accelerators

Better for electrical conductivity (>400°C)

Better for thermal properties  
(higher conductivity, higher heat capacity)

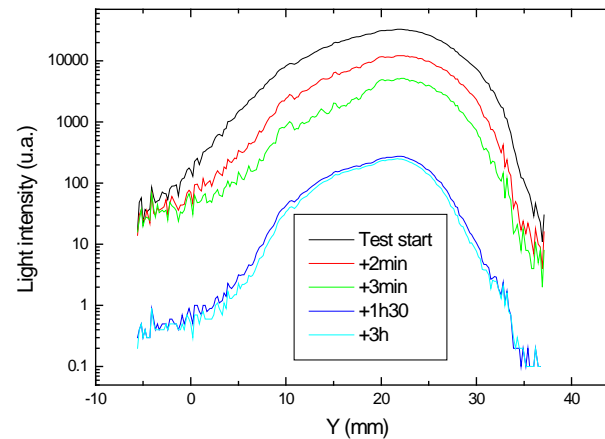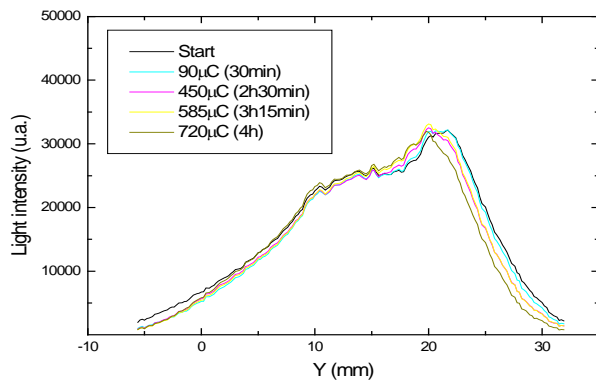




# Degradation of screen

CAS

Degradation clearly visible  
However sensitivity stays essentially  
the same

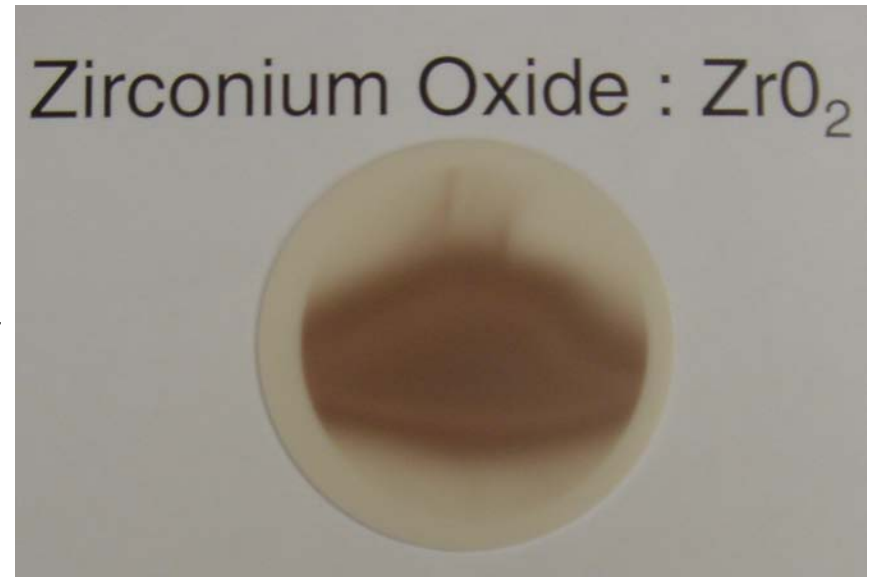




# Screen mechanism

CAS


- Screen with graticule

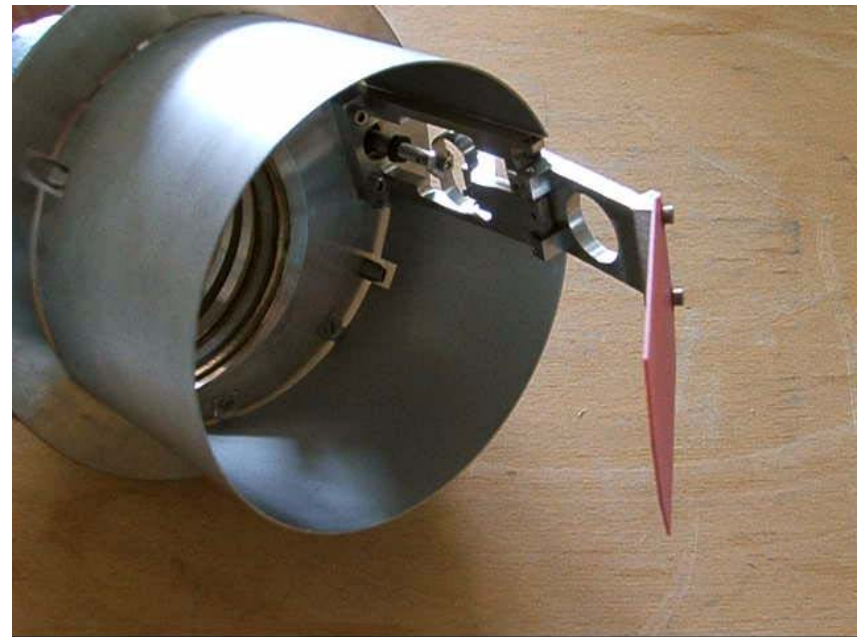




# Results from TV Frame grabber


# CAS

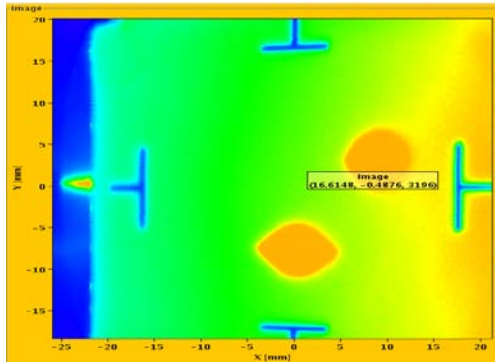

First full turn  
as seen by the  
BTV  
10/9/2008

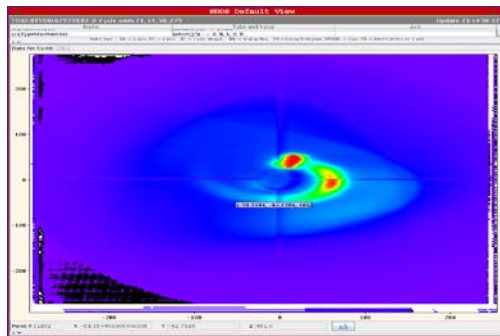

Uncaptured  
beam sweeps  
through the  
dump line

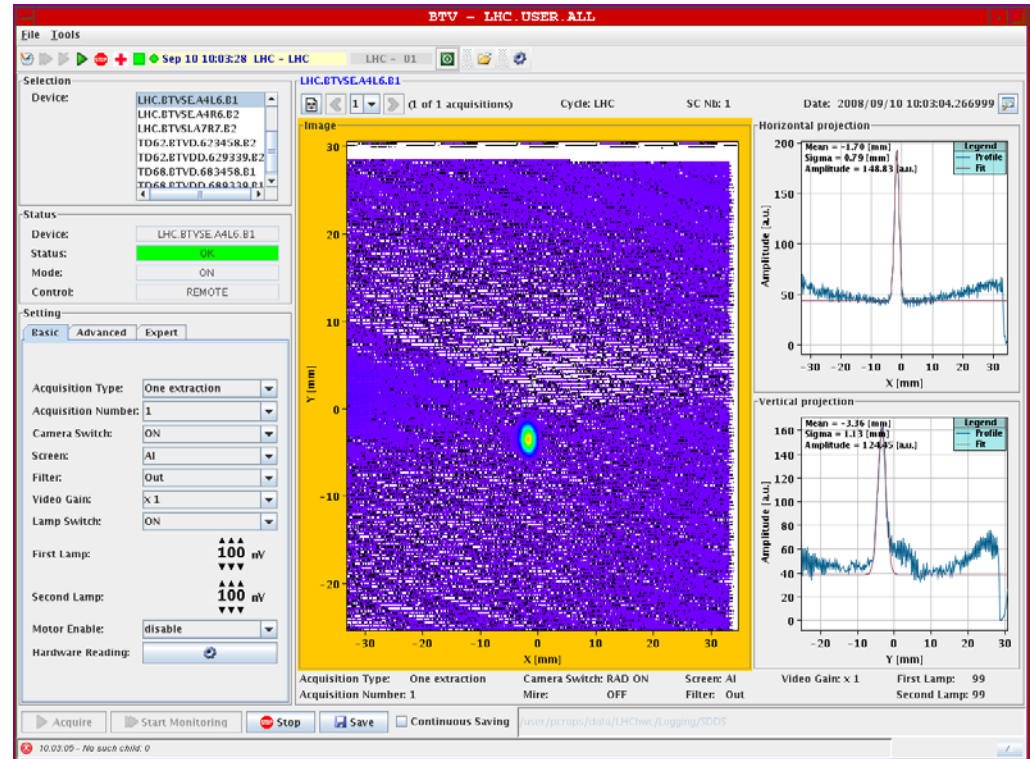

- For further evaluation the video signal is digitized, read-out and treated by program





# Profile measurements



- Secondary emission grids (SEMgrids)

When the beam passes secondary electrons are ejected from the ribbons

The current flowing back onto the ribbons is measured

Electrons are taken away by polarization voltage



One amplifier/ADC chain channel per ribbon






# SEM grids with wires

CAS

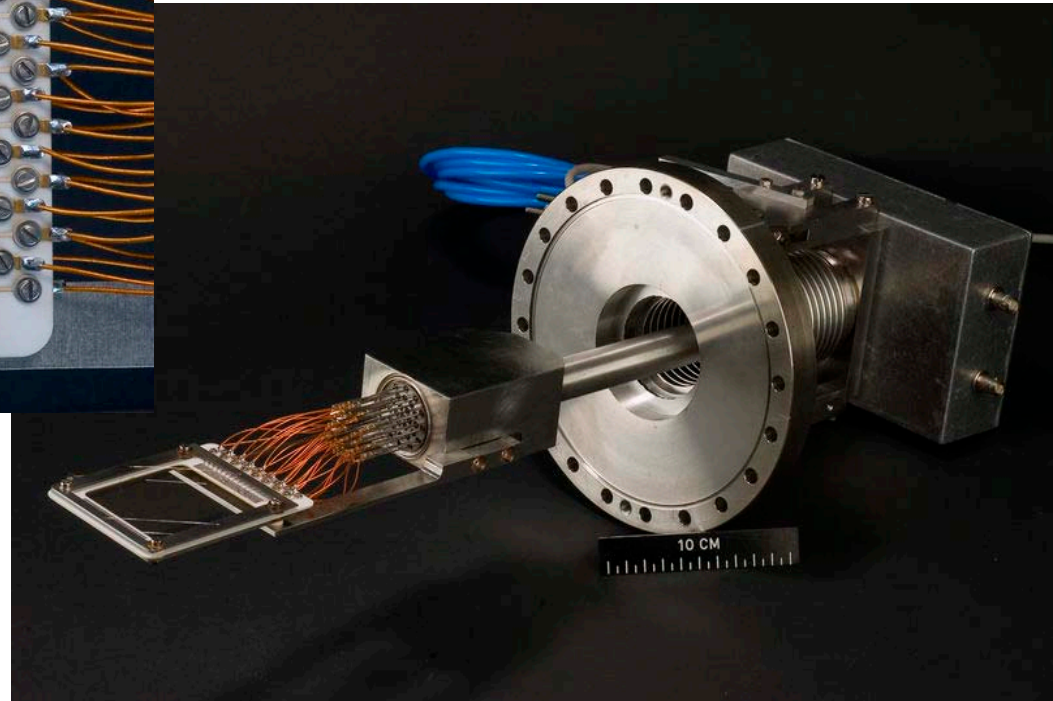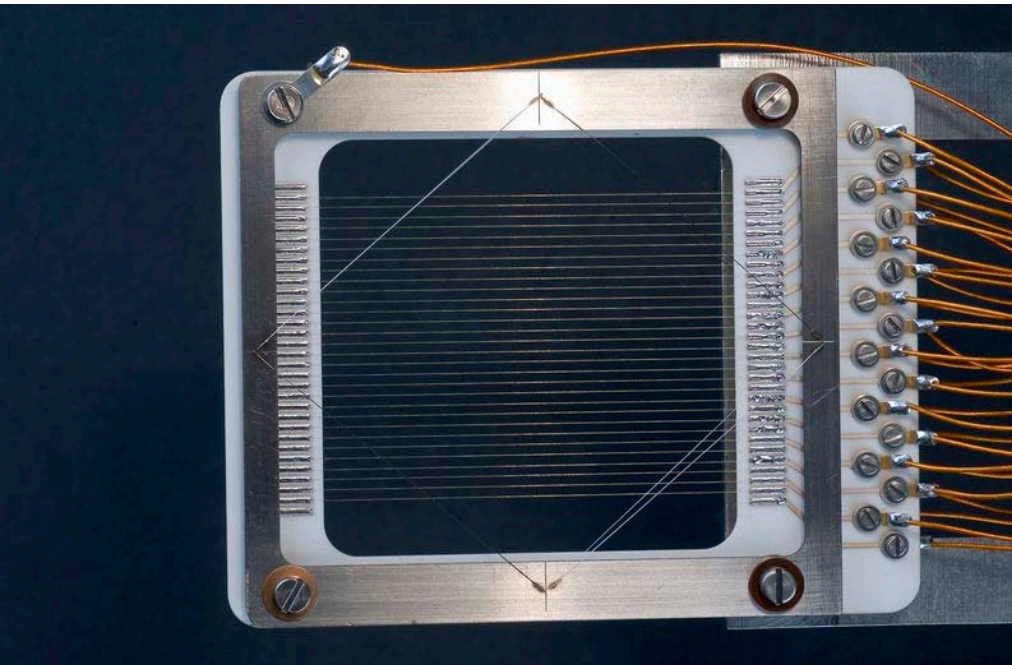



# Profiles from SEMgrids

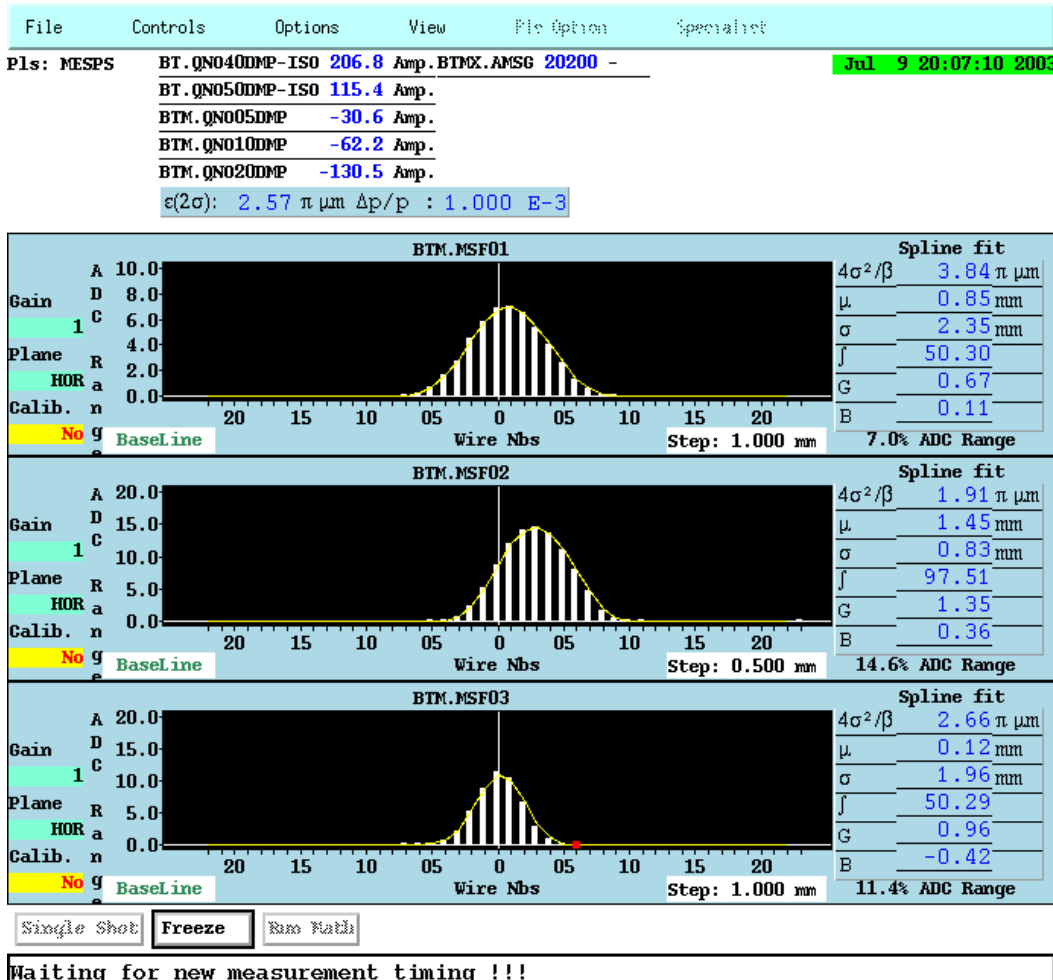

Projection of charge density projected to x or y axis is Measured

One amplifier/ADC per wire  
Large dynamic range

Resolution is given by wire distance

Used only in transfer lines






# Wire Scanners




A thin wire is quickly moved across the beam  
Secondary particle shower is detected outside the vacuum chamber  
on a scintillator/photo-multiplier assembly  
Position and photo-multiplier signal are recorded simultaneously

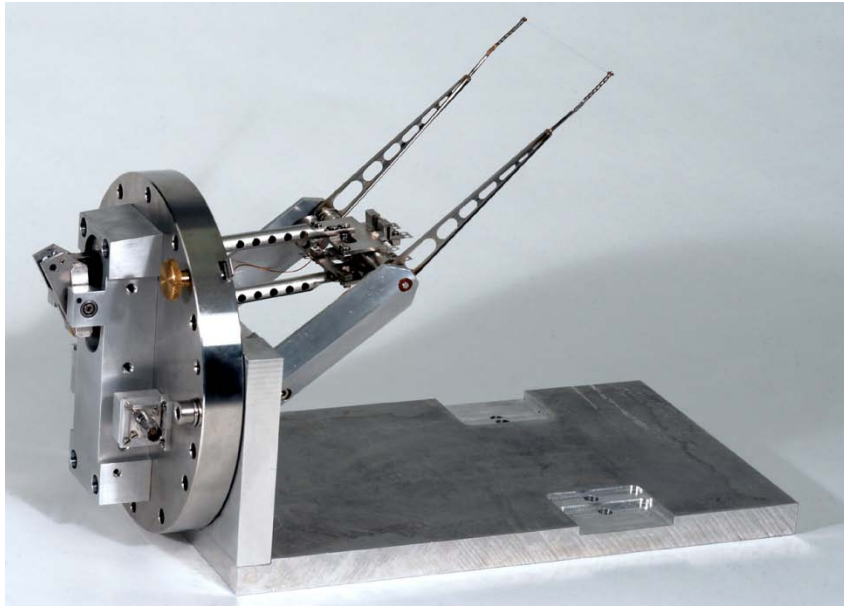



# Wire scanner profile

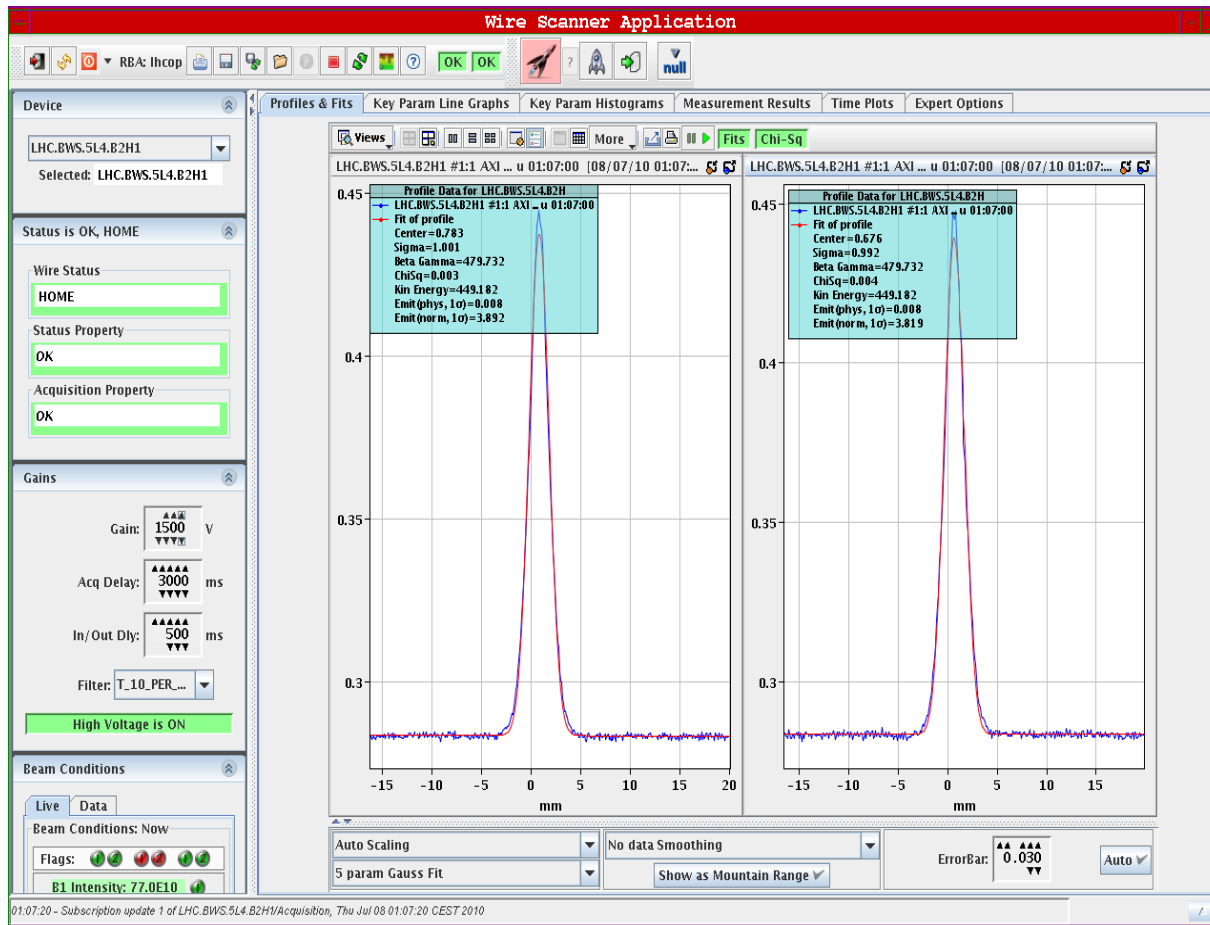

High speed needed because of heating.

Adiabatic damping

Current increase due to Speed increase


Speeds of up to 20m/s  
=> 200g acceleration



# Stored Beam Energies



(Based on graph from R. Schmidt)

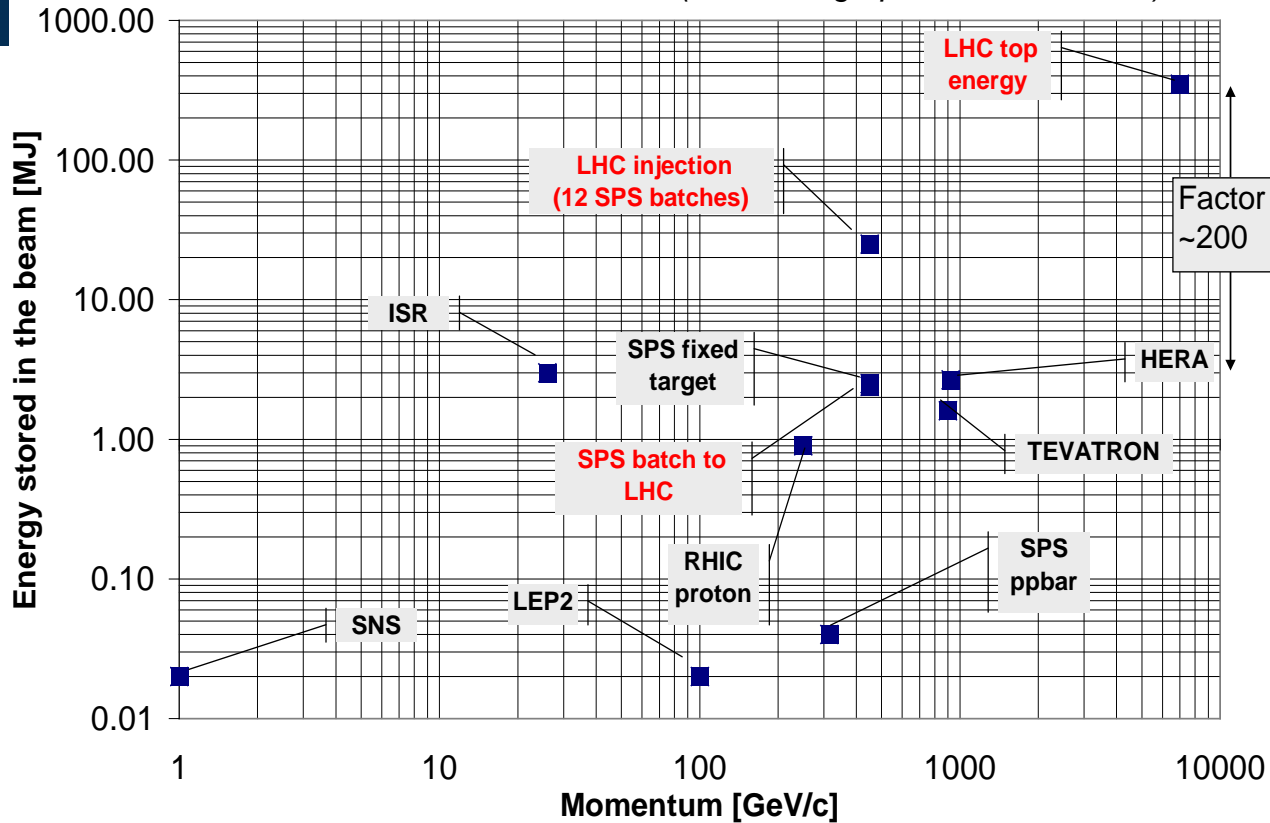

Quench Levels	Units	<i>Tevatron</i>	<i>RHIC</i>	<i>HERA</i>	<i>LHC</i>
<b>Instant loss (0.01 - 10 ms)</b>	[J/cm <sup>3</sup> ]	4.5 10 <sup>-03</sup>	1.8 10 <sup>-02</sup>	2.1 10 <sup>-03</sup> - 6.6 10 <sup>-03</sup>	8.7 10 <sup>-04</sup>
<b>Steady loss (&gt; 100 s)</b>	[W/cm <sup>3</sup> ]	7.5 10 <sup>-02</sup>	7.5 10 <sup>-02</sup>		5.3 10 <sup>-03</sup>





# Beam power in the LHC

CAS




The Linac beam (160 mA, 200 $\mu$ s, 50 MeV, 1Hz) is enough to burn a hole into the vacuum chamber

What about the LHC beam: 2808 bunches of  $15 \cdot 10^{11}$  particles at 7 TeV?  
1 bunch corresponds to a 5 kg bullet at 800 km/h



# Beam Dammage

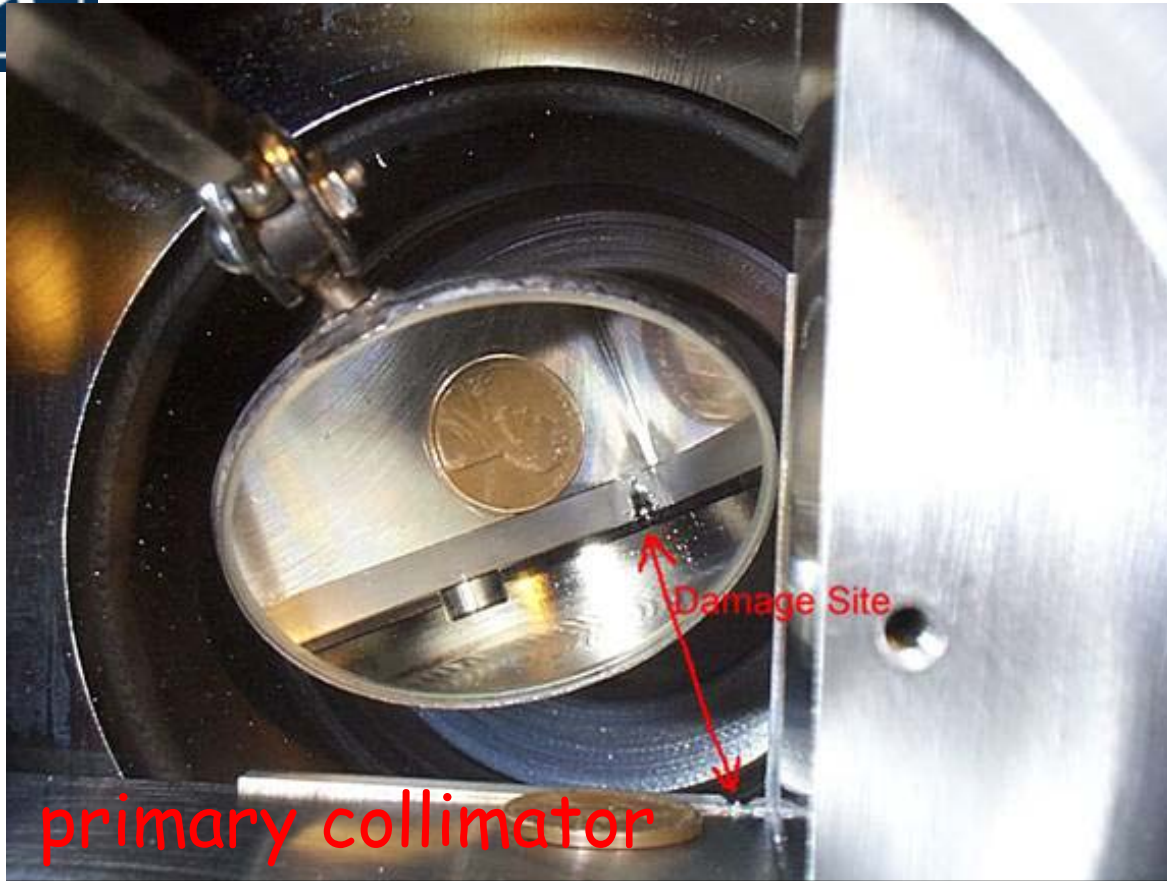

Fermi Lab's Tevatron has 200 times less beam power than LHC!



# Beam Loss Monitor Types

CAS

- Design criteria: Signal speed and robustness
- Dynamic range ( $> 10^9$ ) limited by leakage current through insulator ceramics (lower) and saturation due to space charge (upper limit).

## Secondary Emission Monitor

(SEM):

- Length 10 cm
- $P < 10^{-7}$  bar
- $\sim 30000$  times smaller gain



## Ionization chamber:


- $N_2$  gas filling at 100 mbar over-pressure
- Length 50 cm
- Sensitive volume 1.5 l
- Ion collection time 85  $\mu$ s

- Both monitors:
  - Parallel electrodes (Al, SEM: Ti) separated by 0.5 cm
  - Low pass filter at the HV input
  - Voltage 1.5 kV





# Quench levels

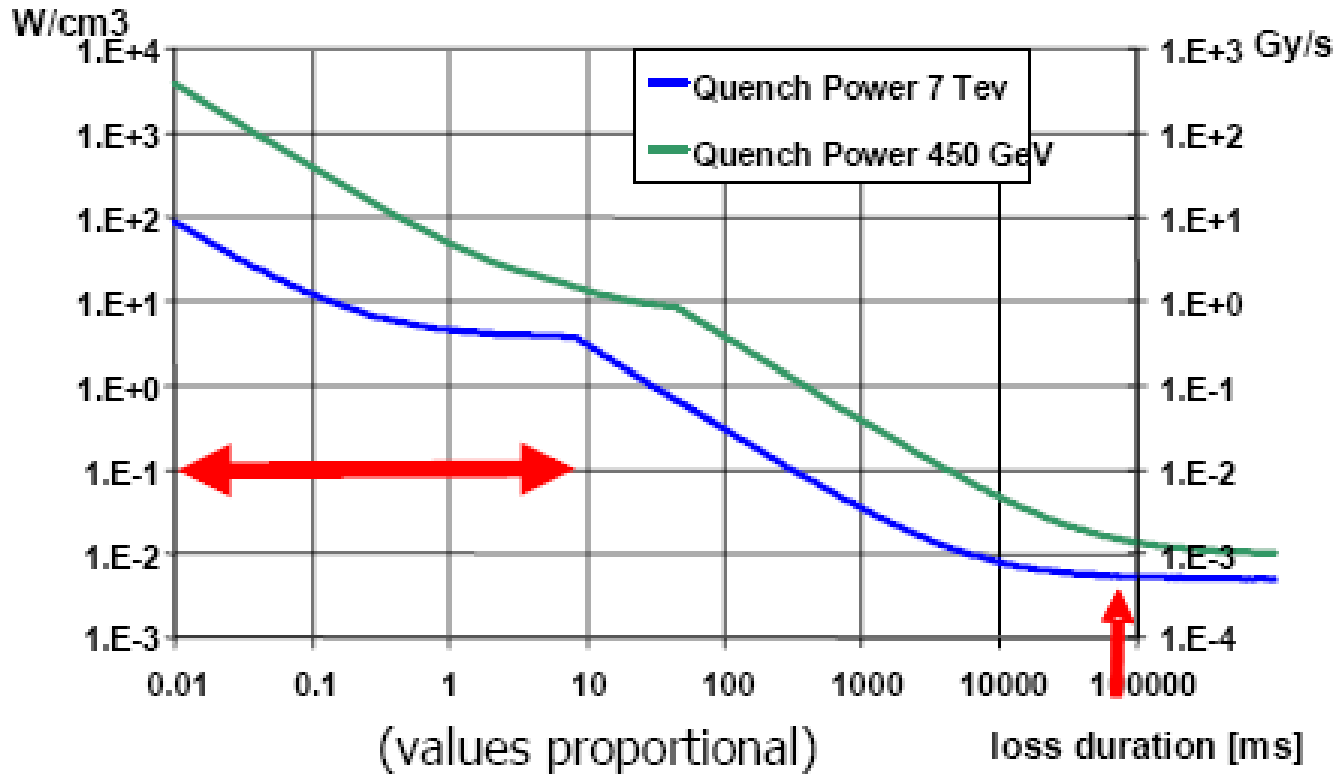






# Industrial production of chambers

CAS

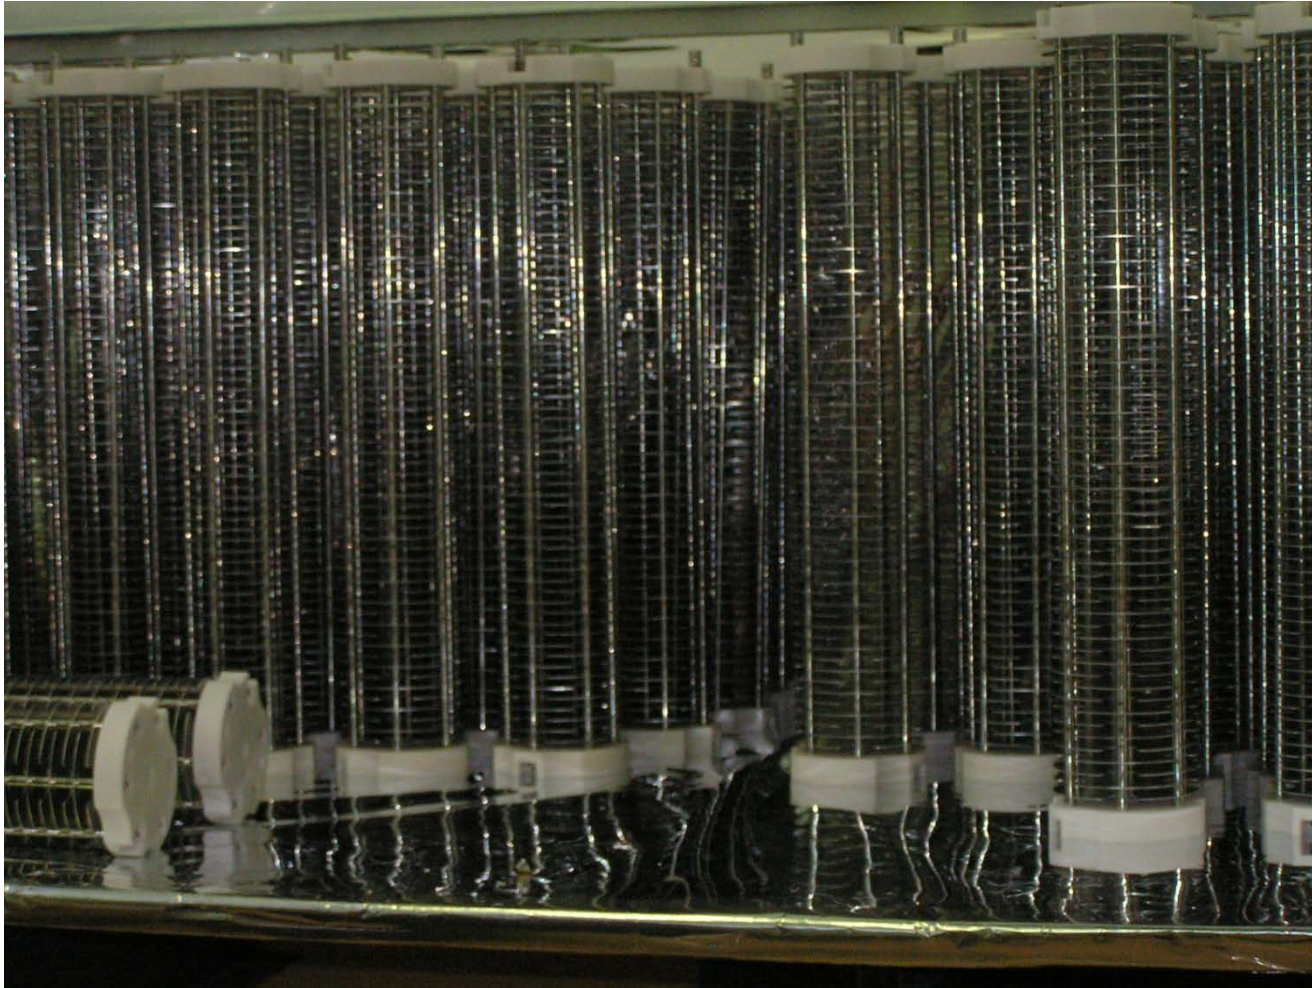


Beam loss must be measured all around the ring  
=> 4000 sensors!



# System layout

CAS

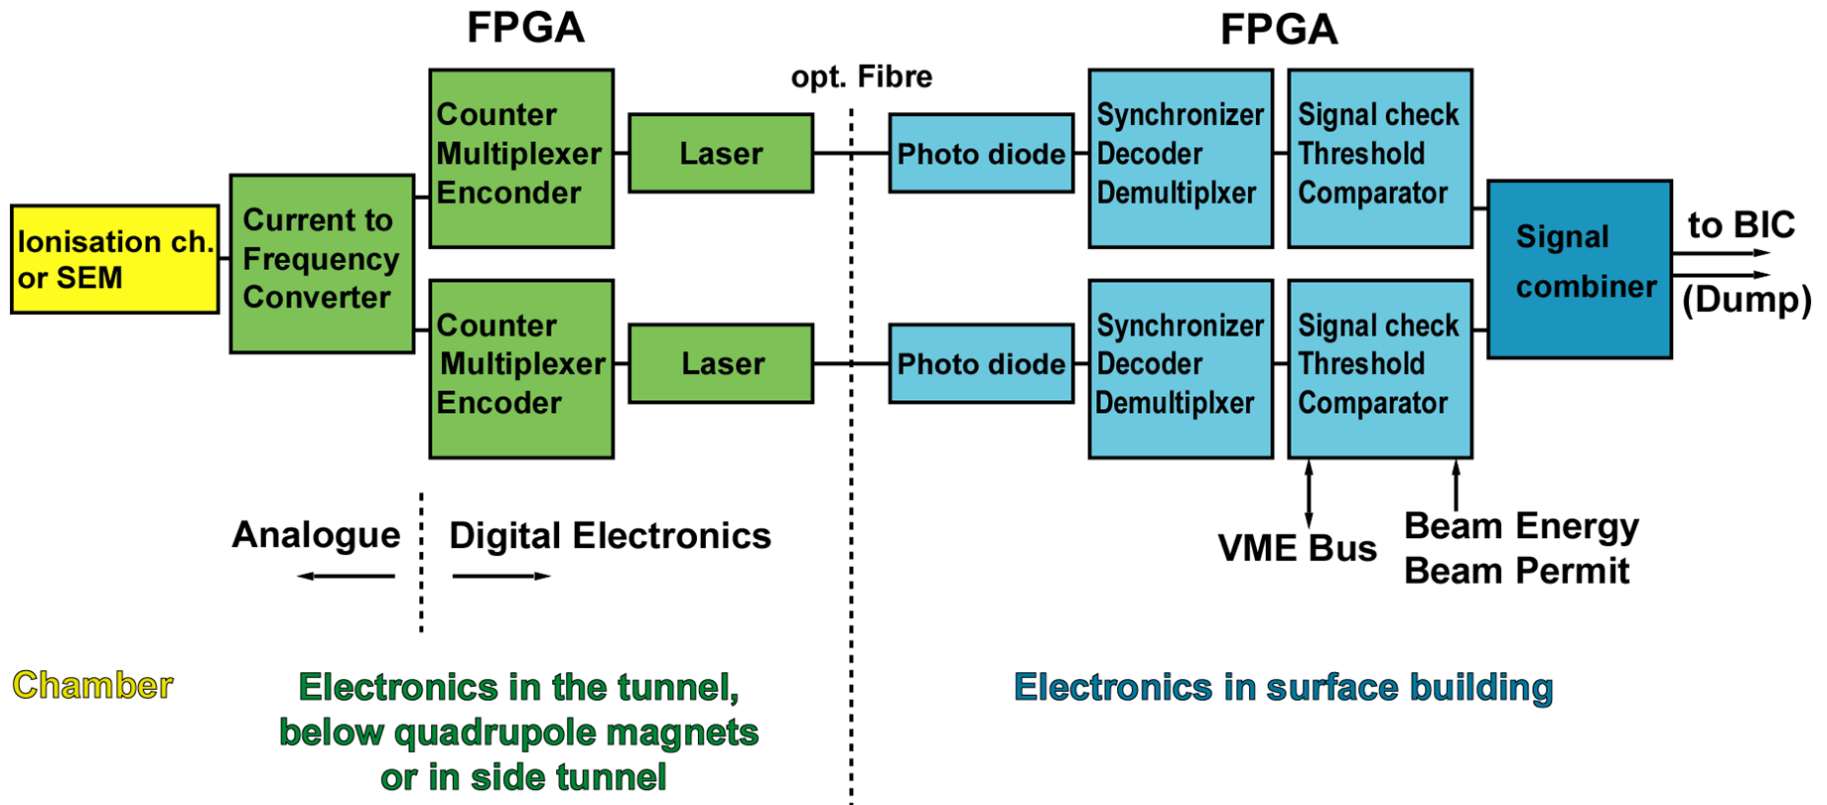





# Successive running sums

CAS

